

This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

**As rescanning documents *will not* correct images,
please do not report the images to the
Image Problem Mailbox.**

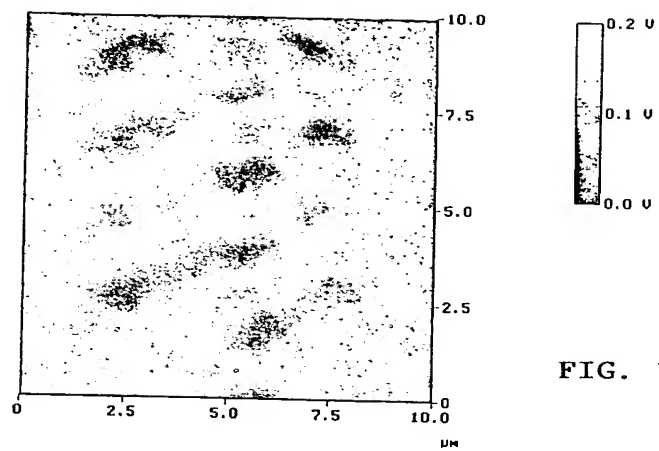


FIG. 1A

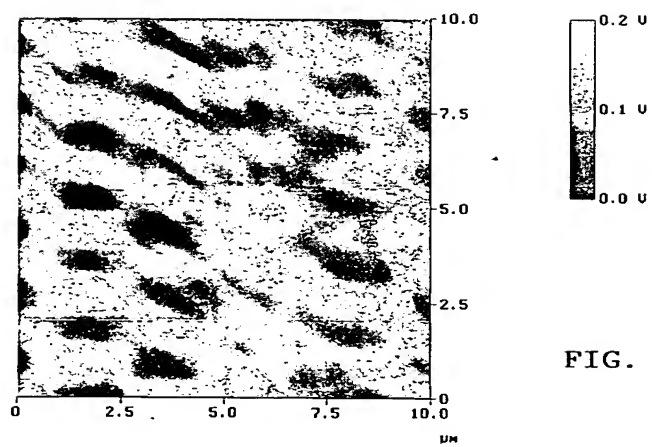


FIG. 1B

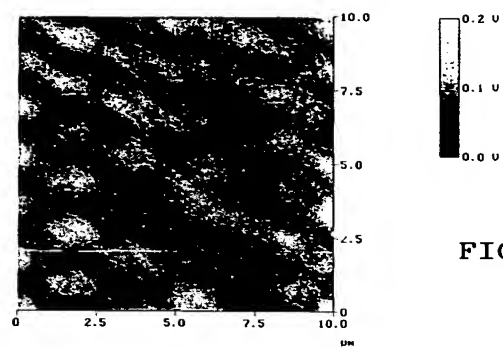


FIG. 2A

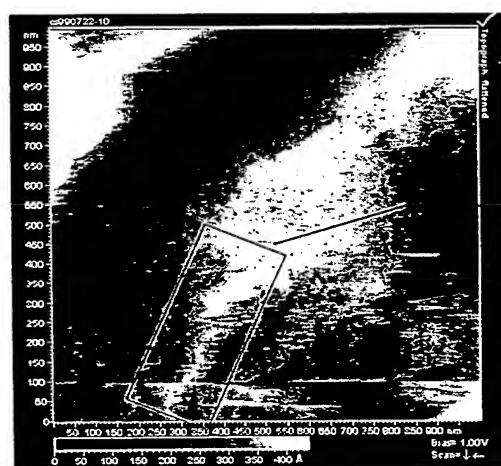


FIG. 2B

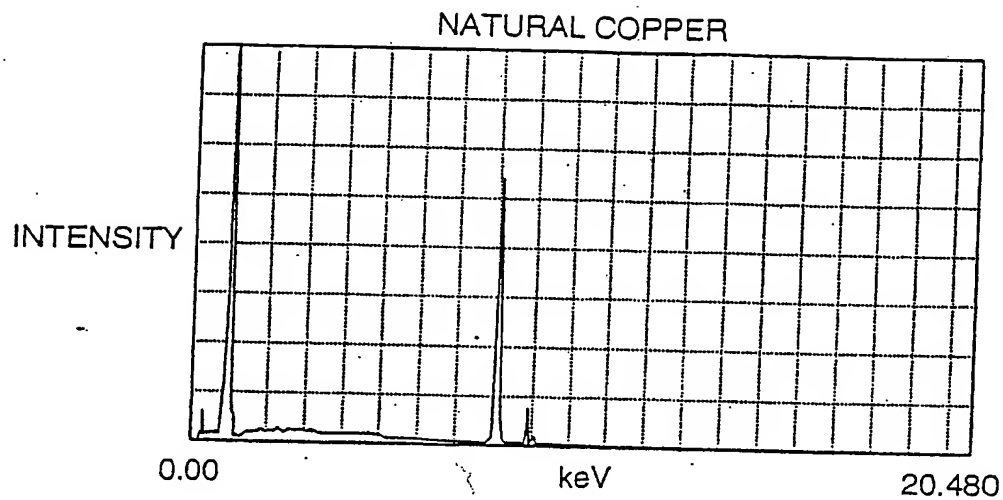


FIG. 3A

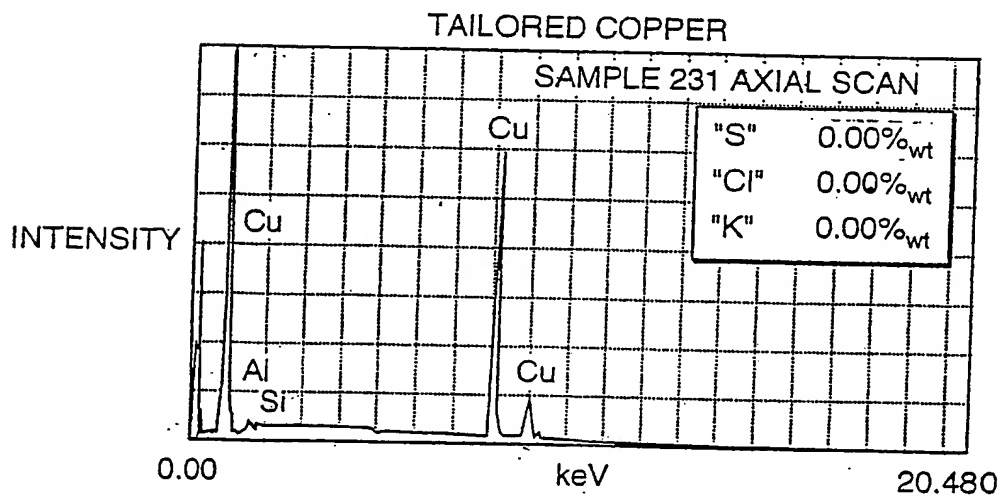


FIG. 3B

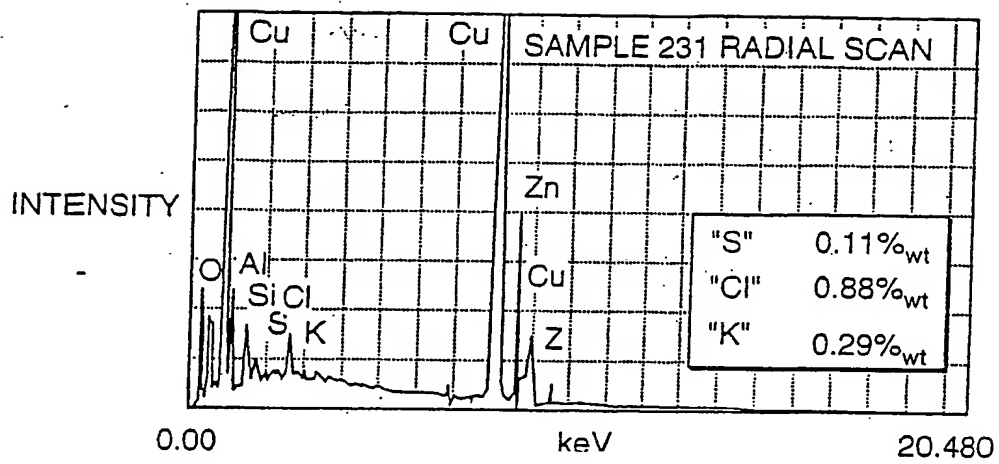


FIG. 4A


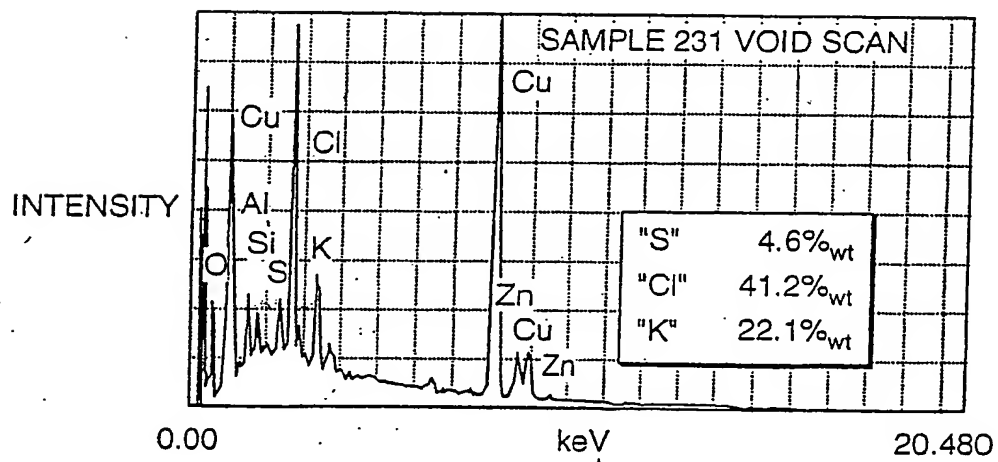


FIG. 4B

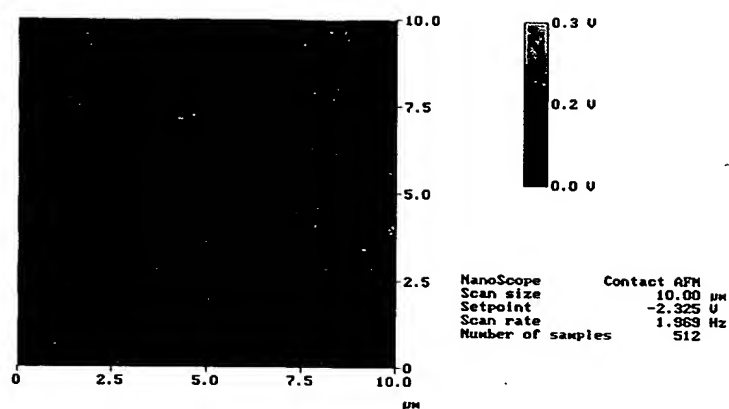

p1990722.037

MFM: Sample 231 Void Scan

FIG. 5A

TAILORED COPPER

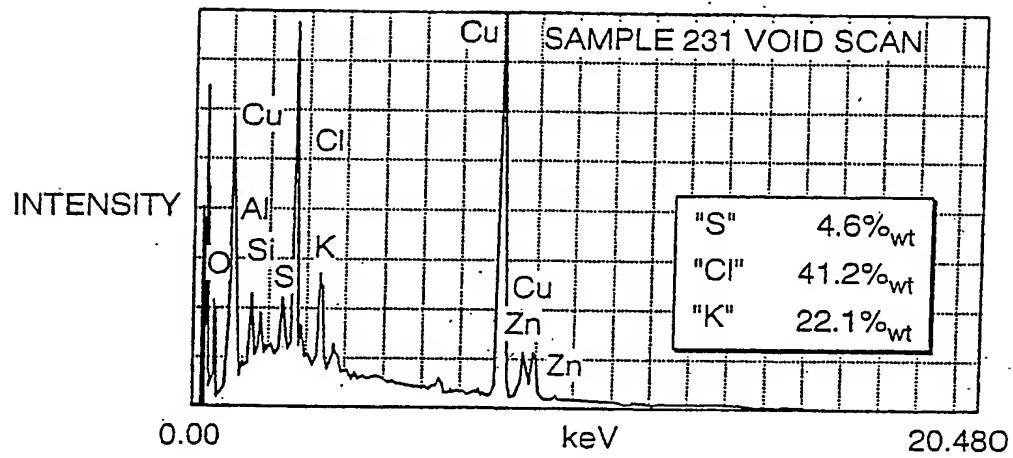


FIG. 5B

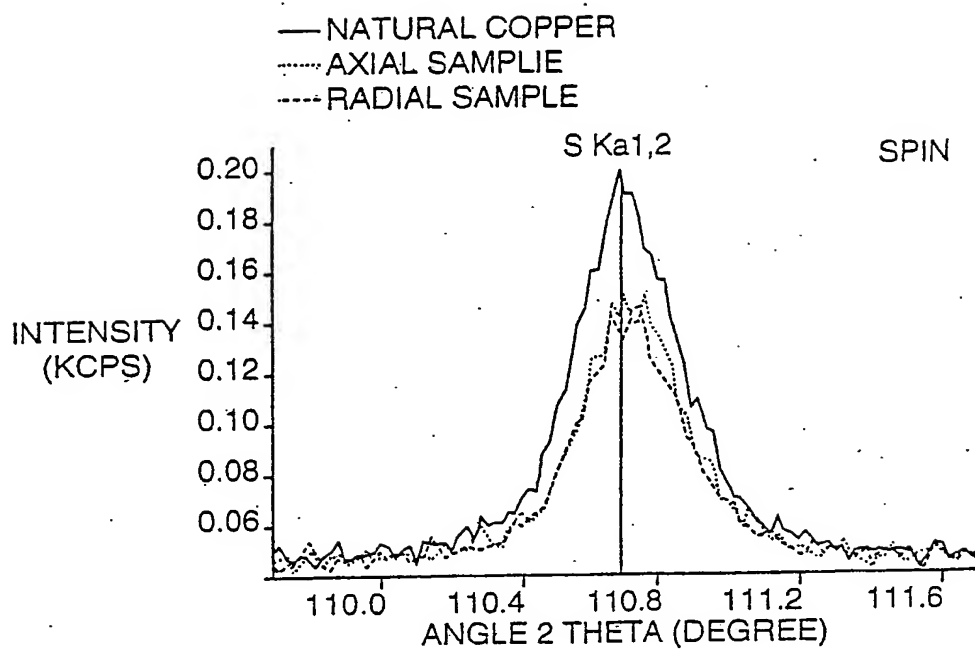


FIG. 6A


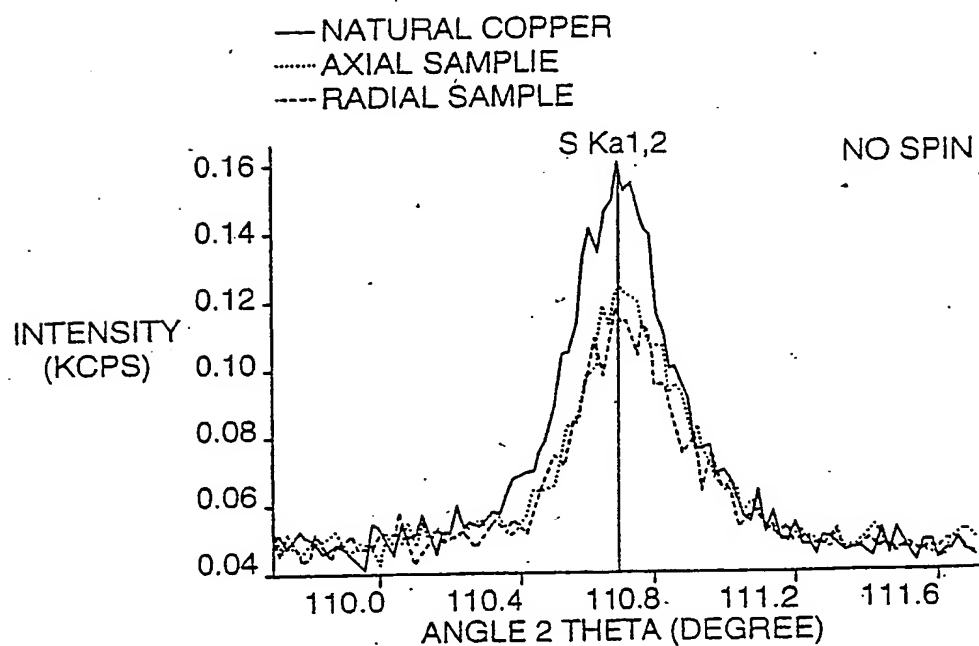


FIG. 6B

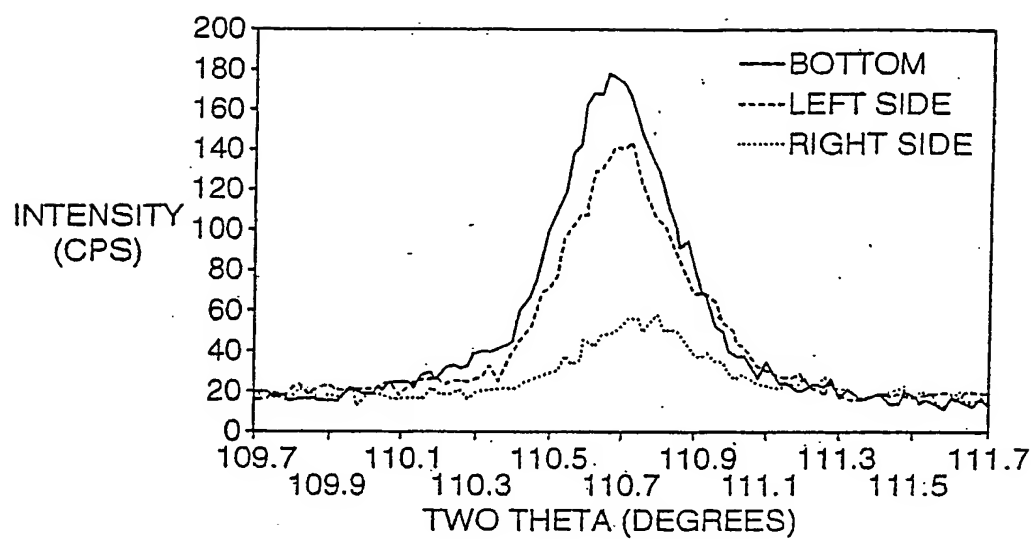

XRF ANALYSIS

FIG. 7

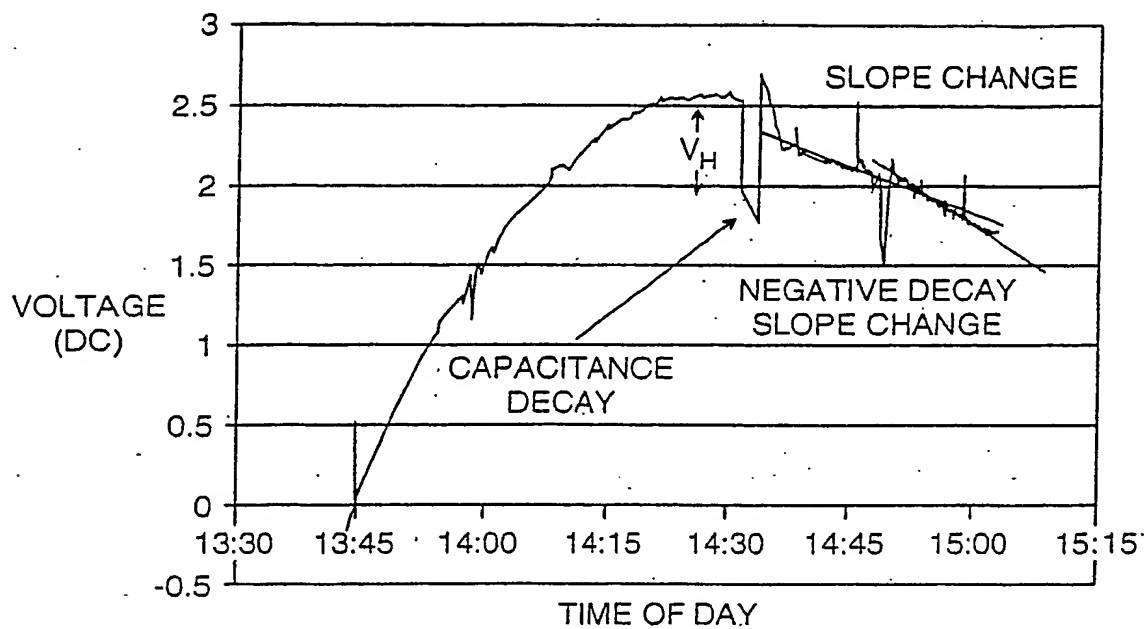


FIG. 8

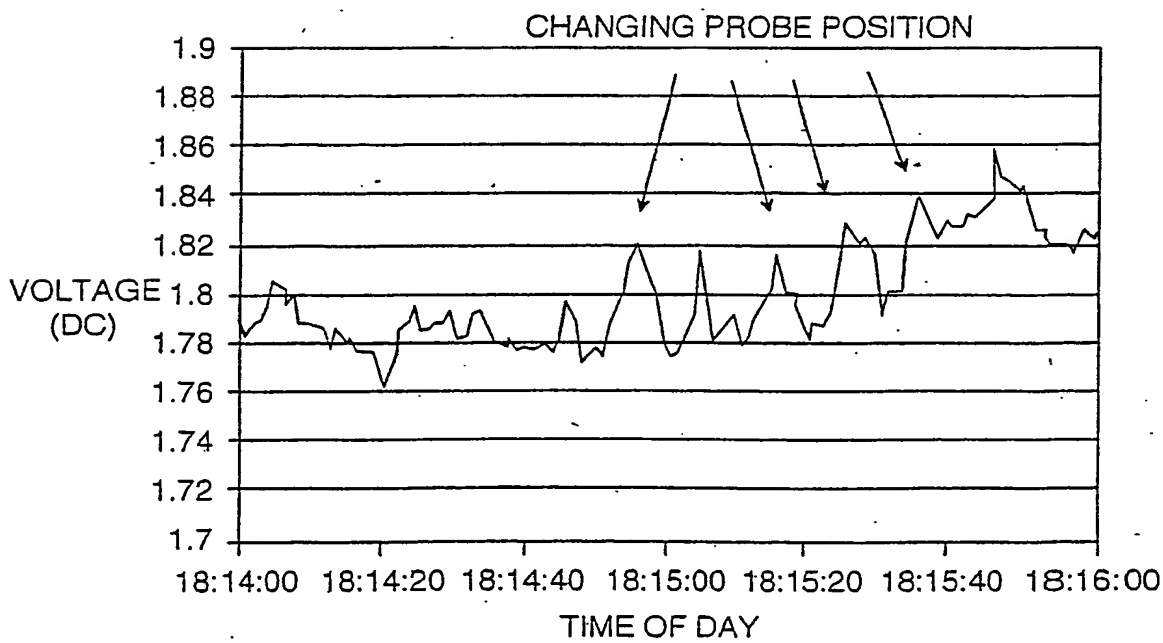


FIG. 9

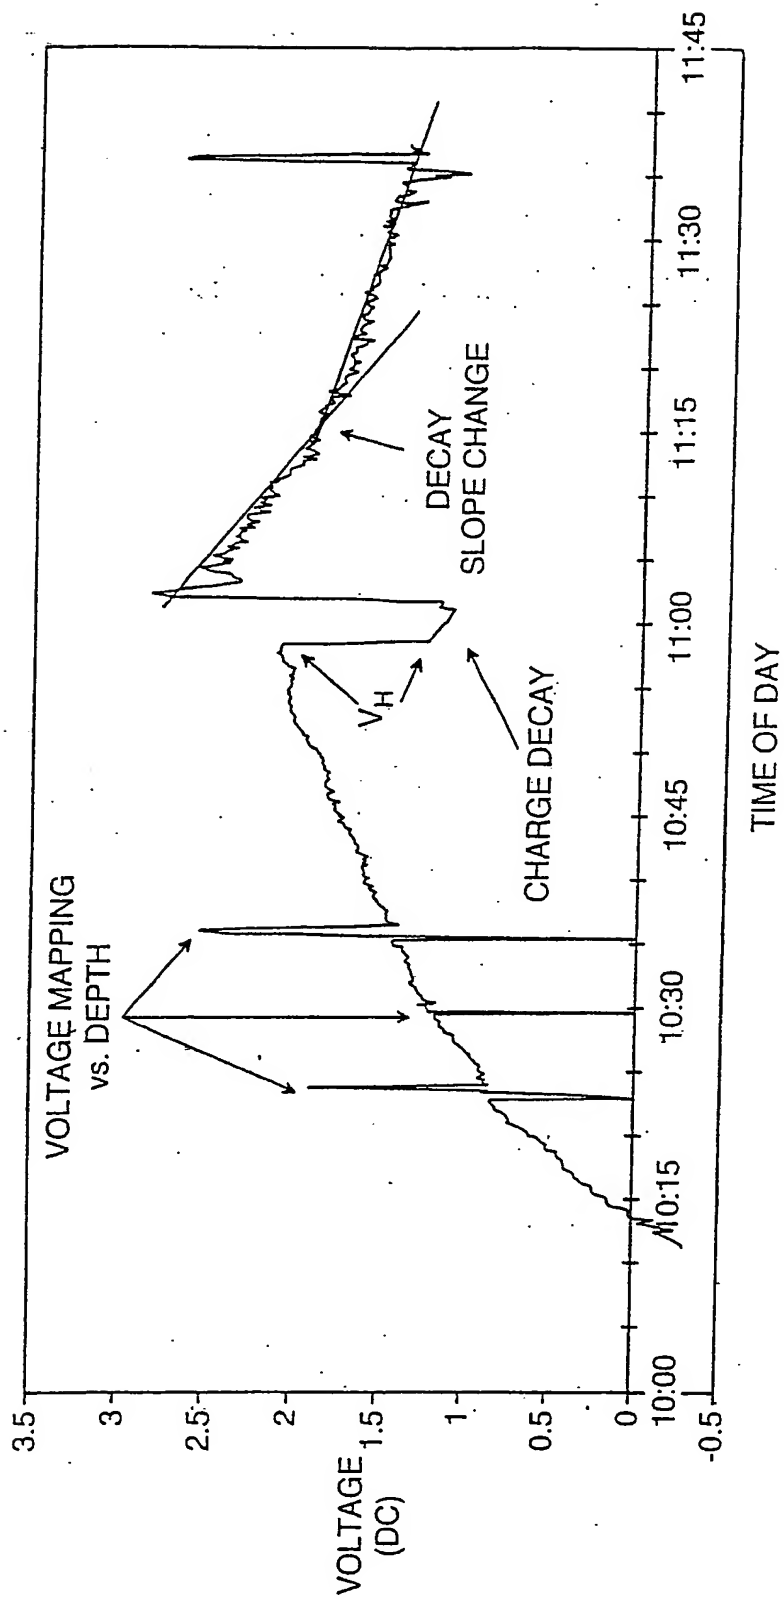


FIG. 10

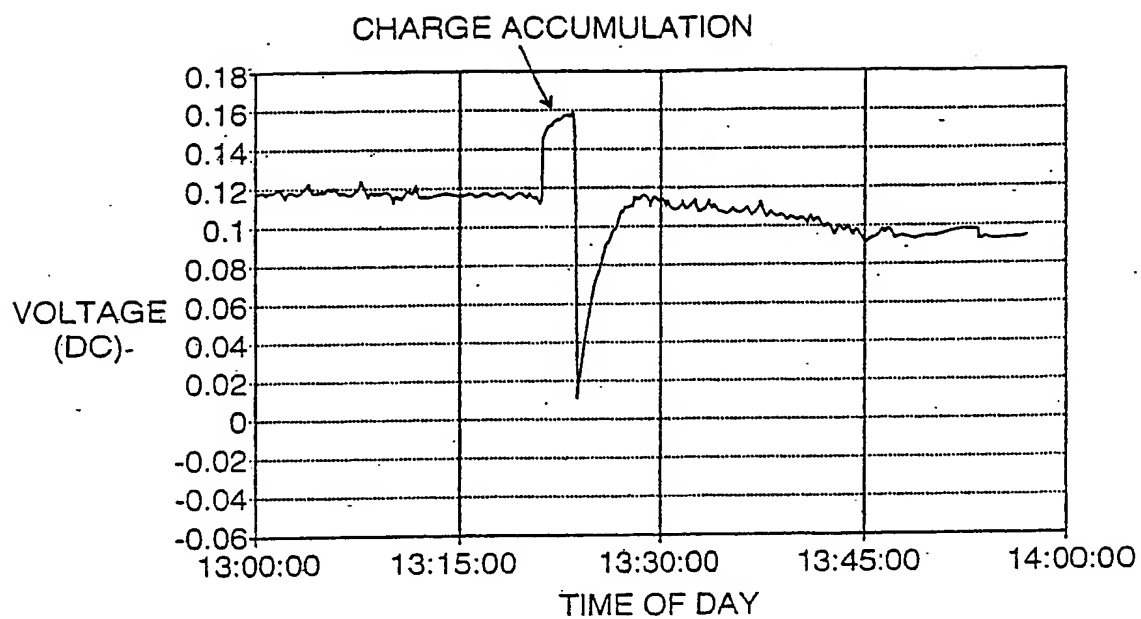


FIG. 11

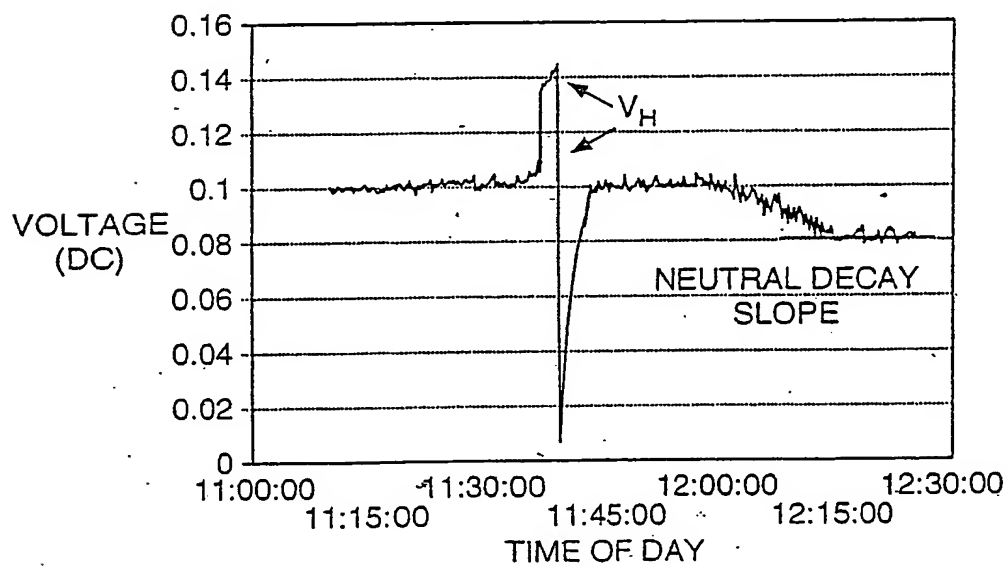


FIG. 12

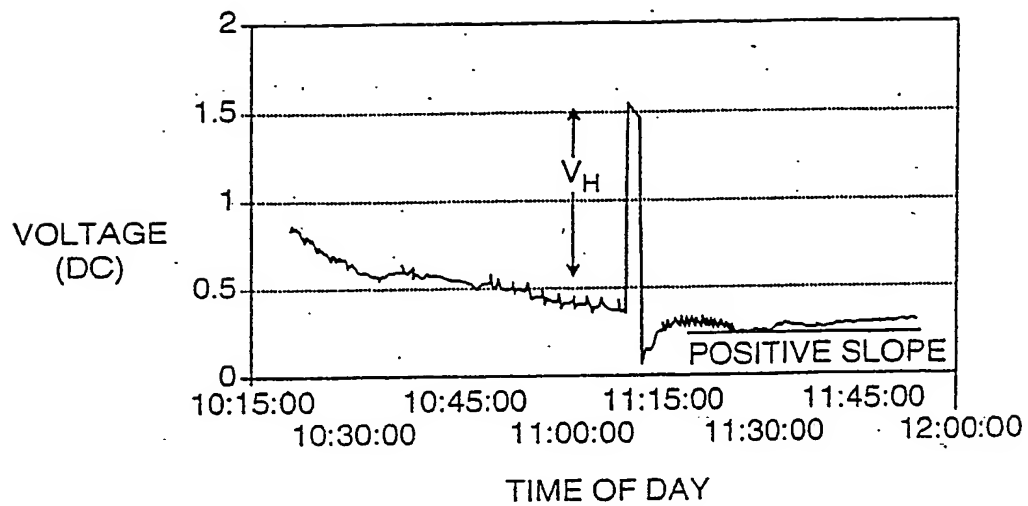


FIG. 13

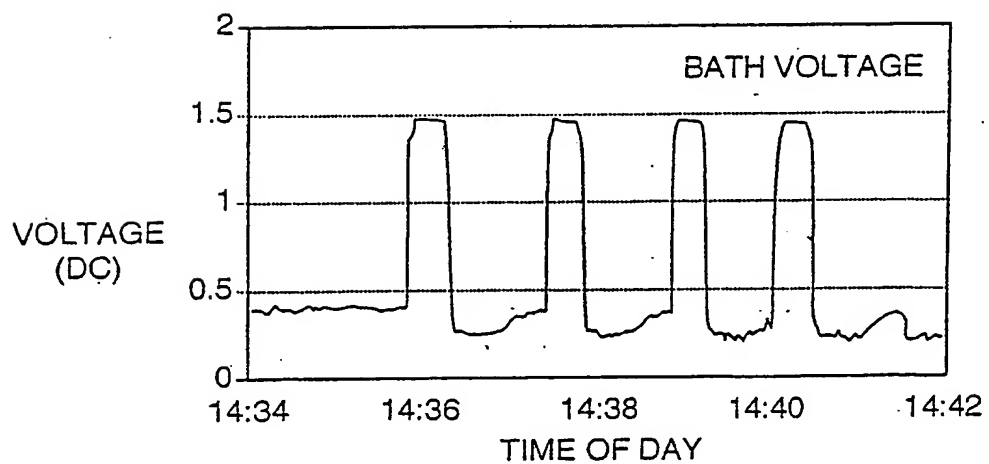


FIG. 14

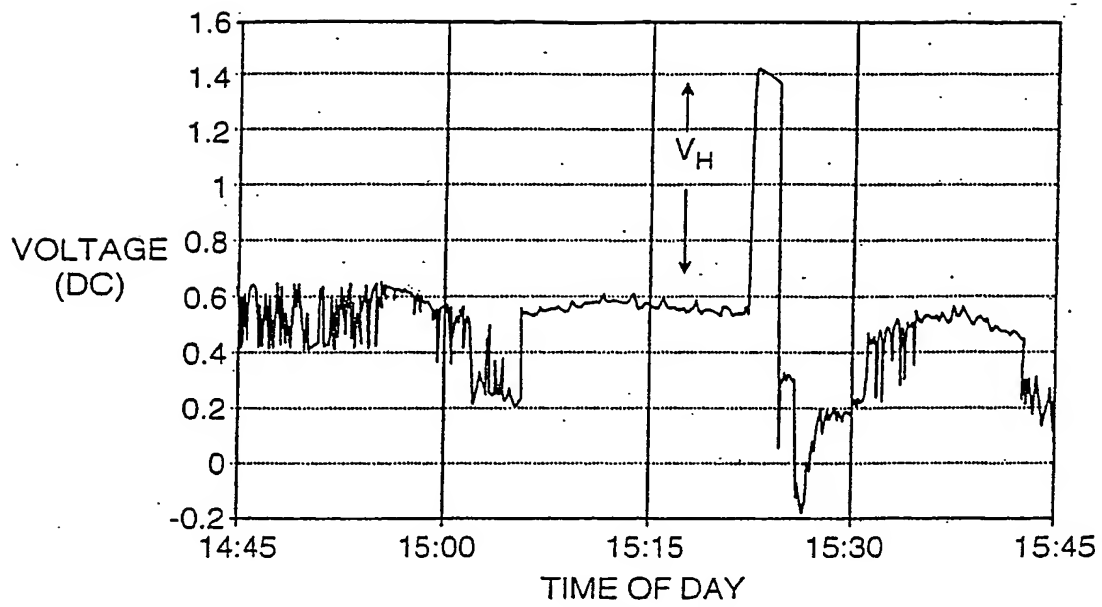


FIG. 15

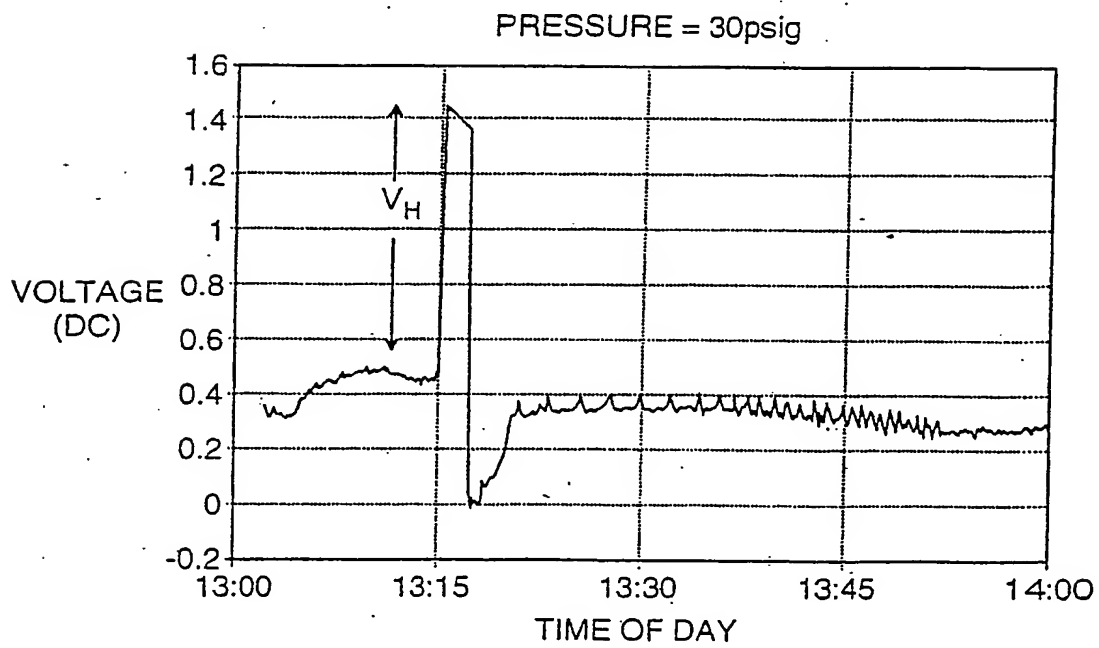


FIG. 16

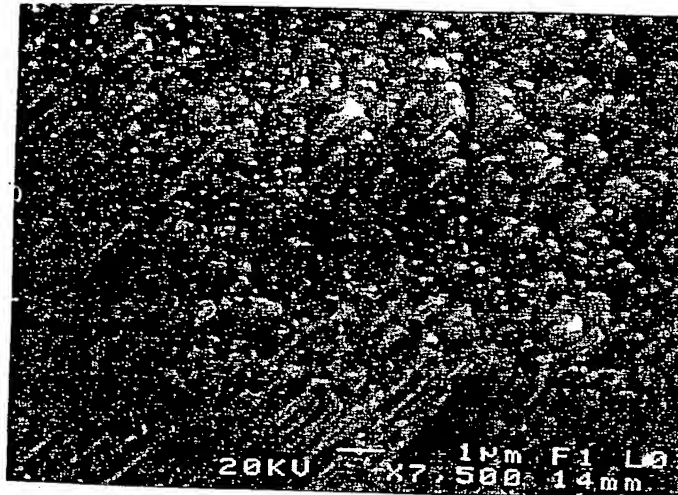


FIG. 17A

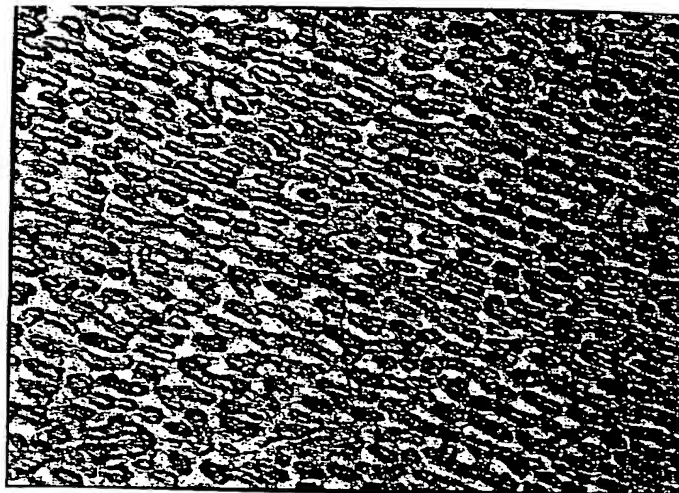


FIG. 17B

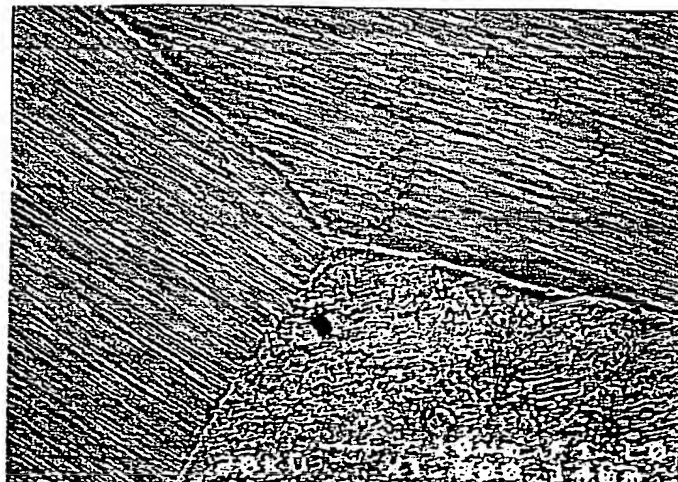


FIG. 17C

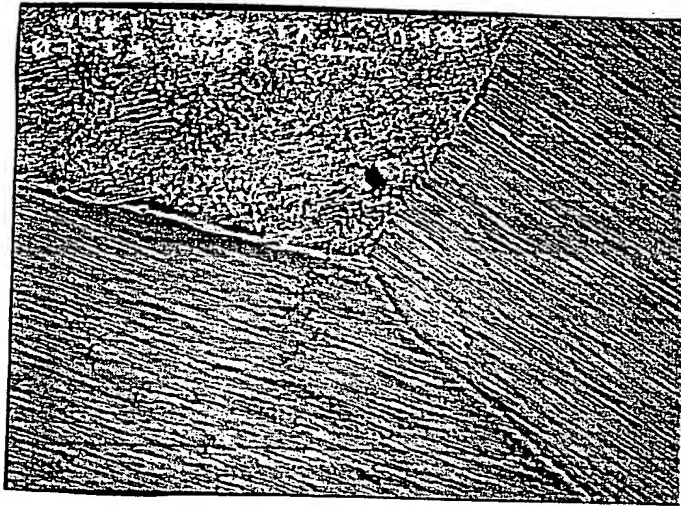


FIG. 18A

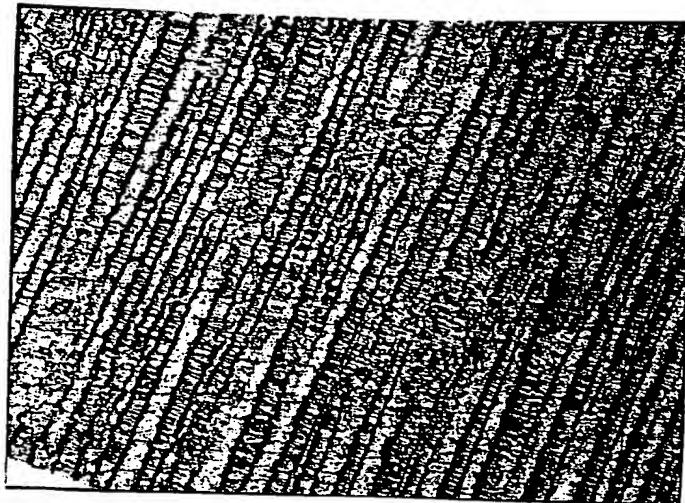


FIG. 18B

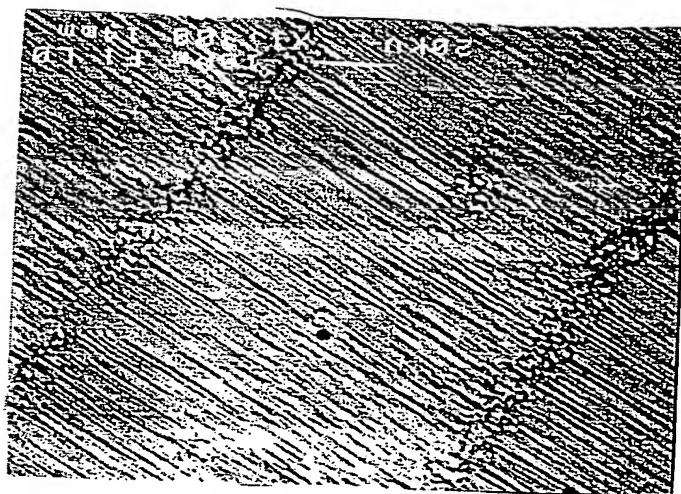


FIG. 18C

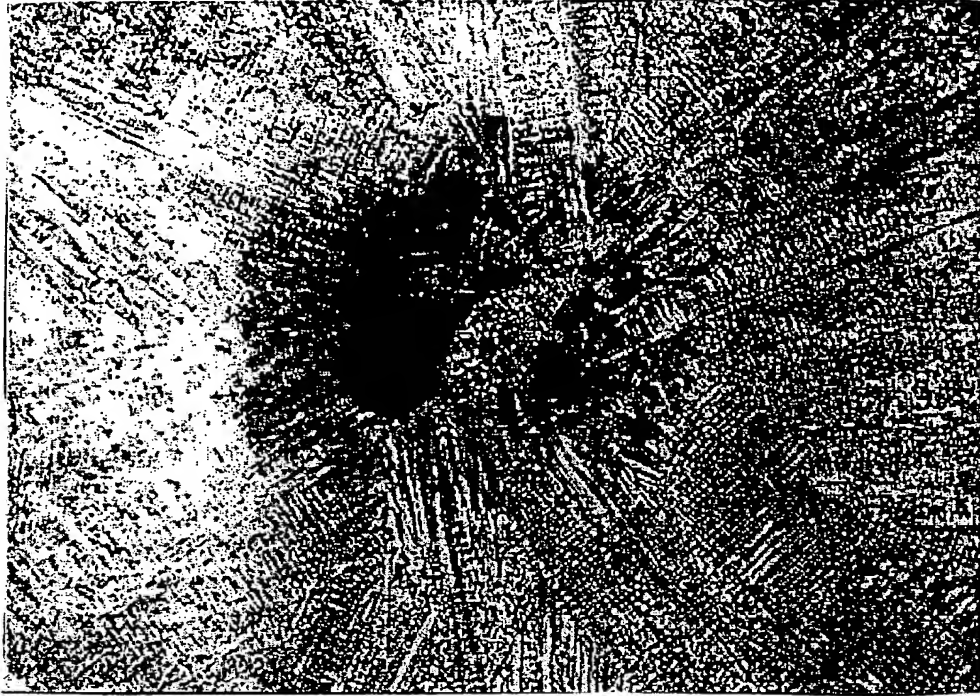


FIG. 19A

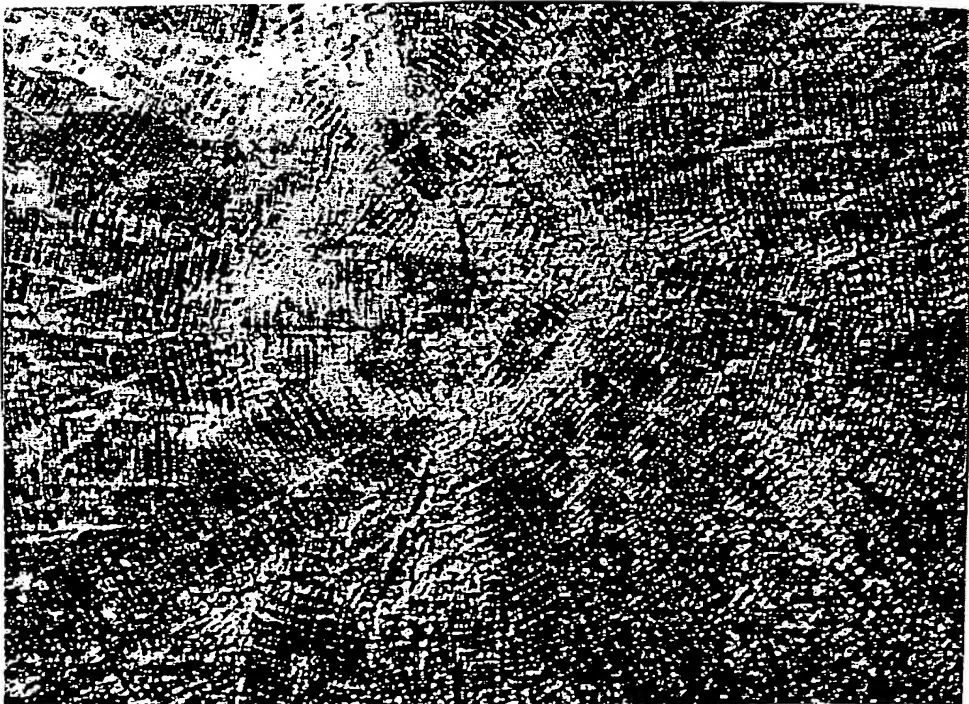


FIG. 19B

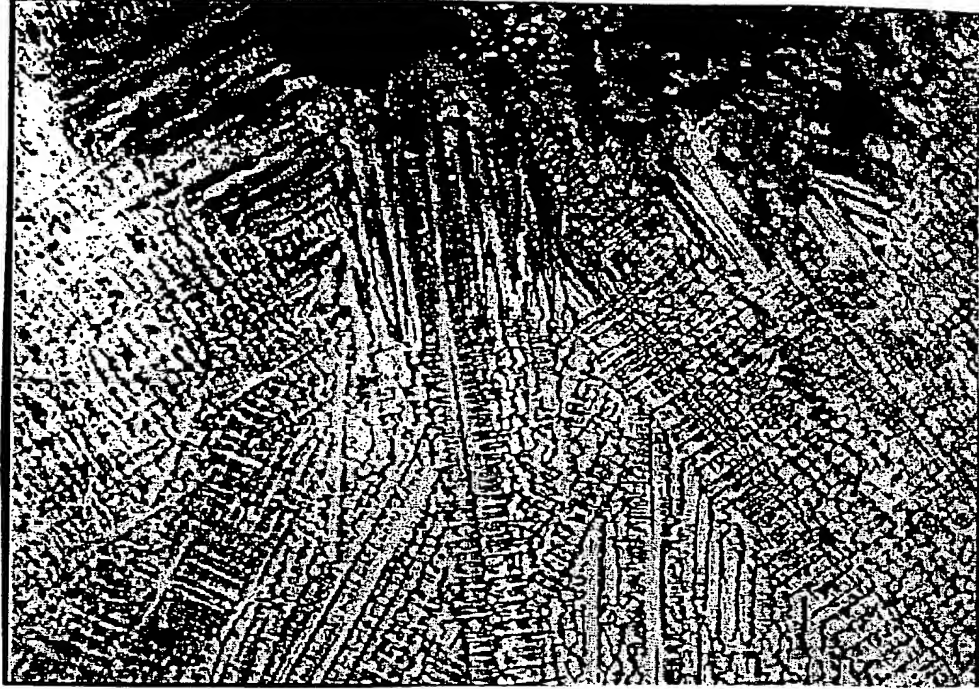


FIG. 20A



FIG. 20B

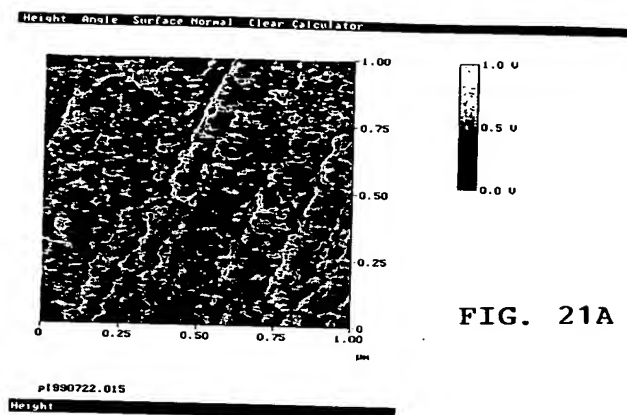


FIG. 21A

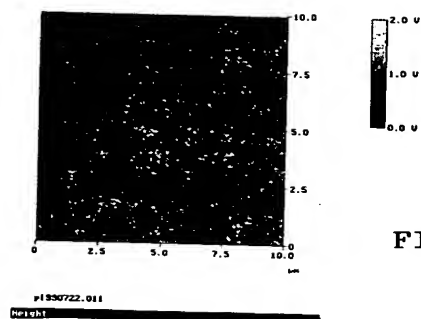


FIG. 21B

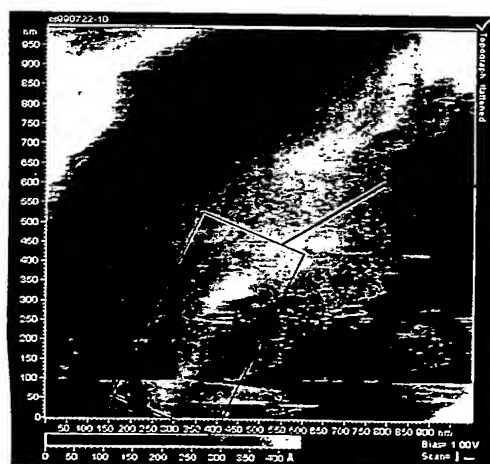


FIG. 21C

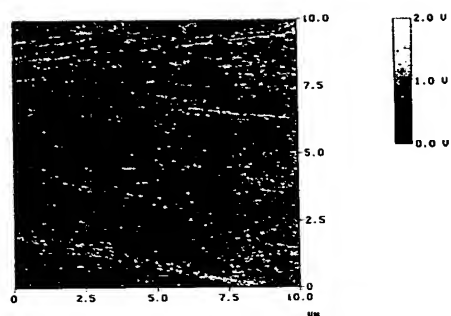


FIG. 22A

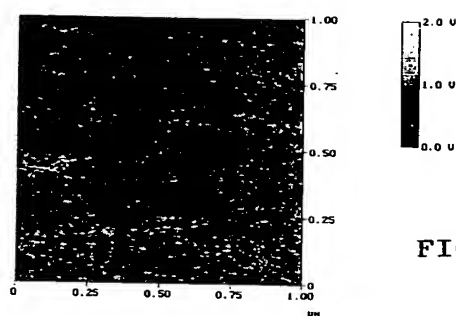


FIG. 22B

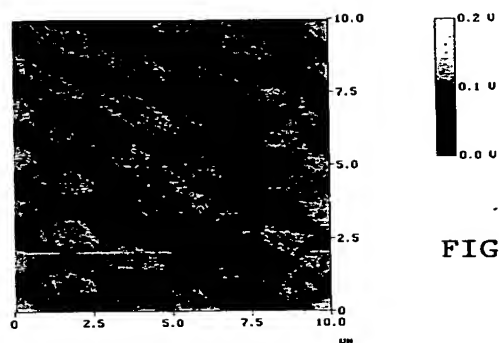


FIG. 22C

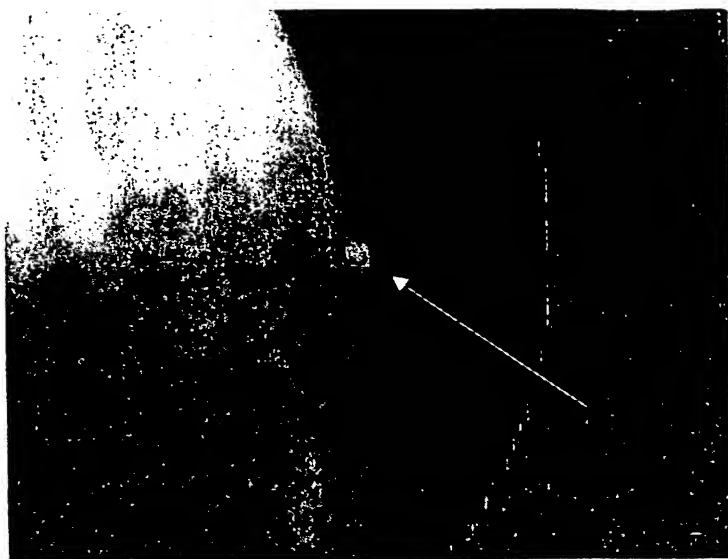



FIG. 23A



FIG. 23B



FIG. 23C

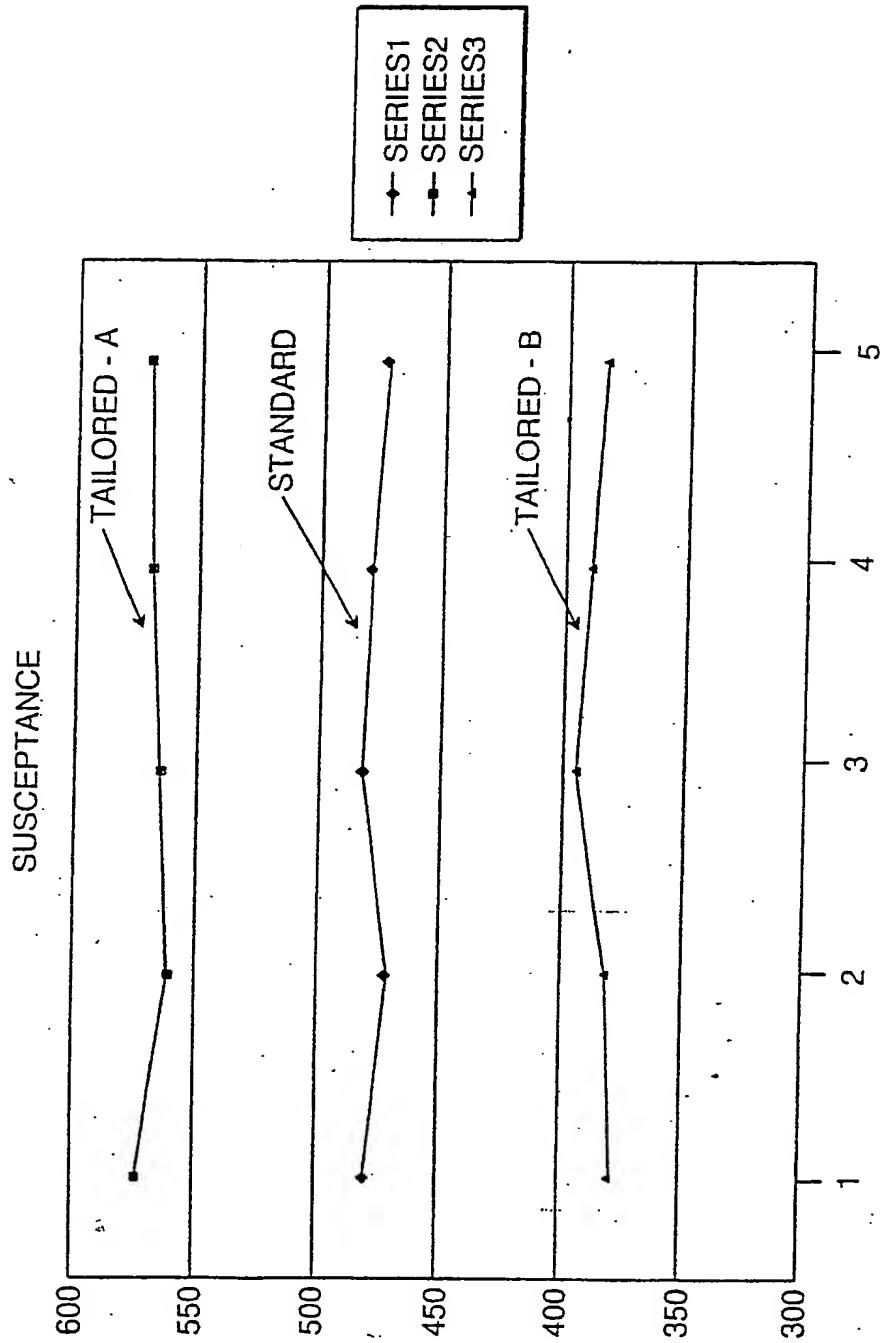

14-01-01 scans for Copper (LiF220/FPC)

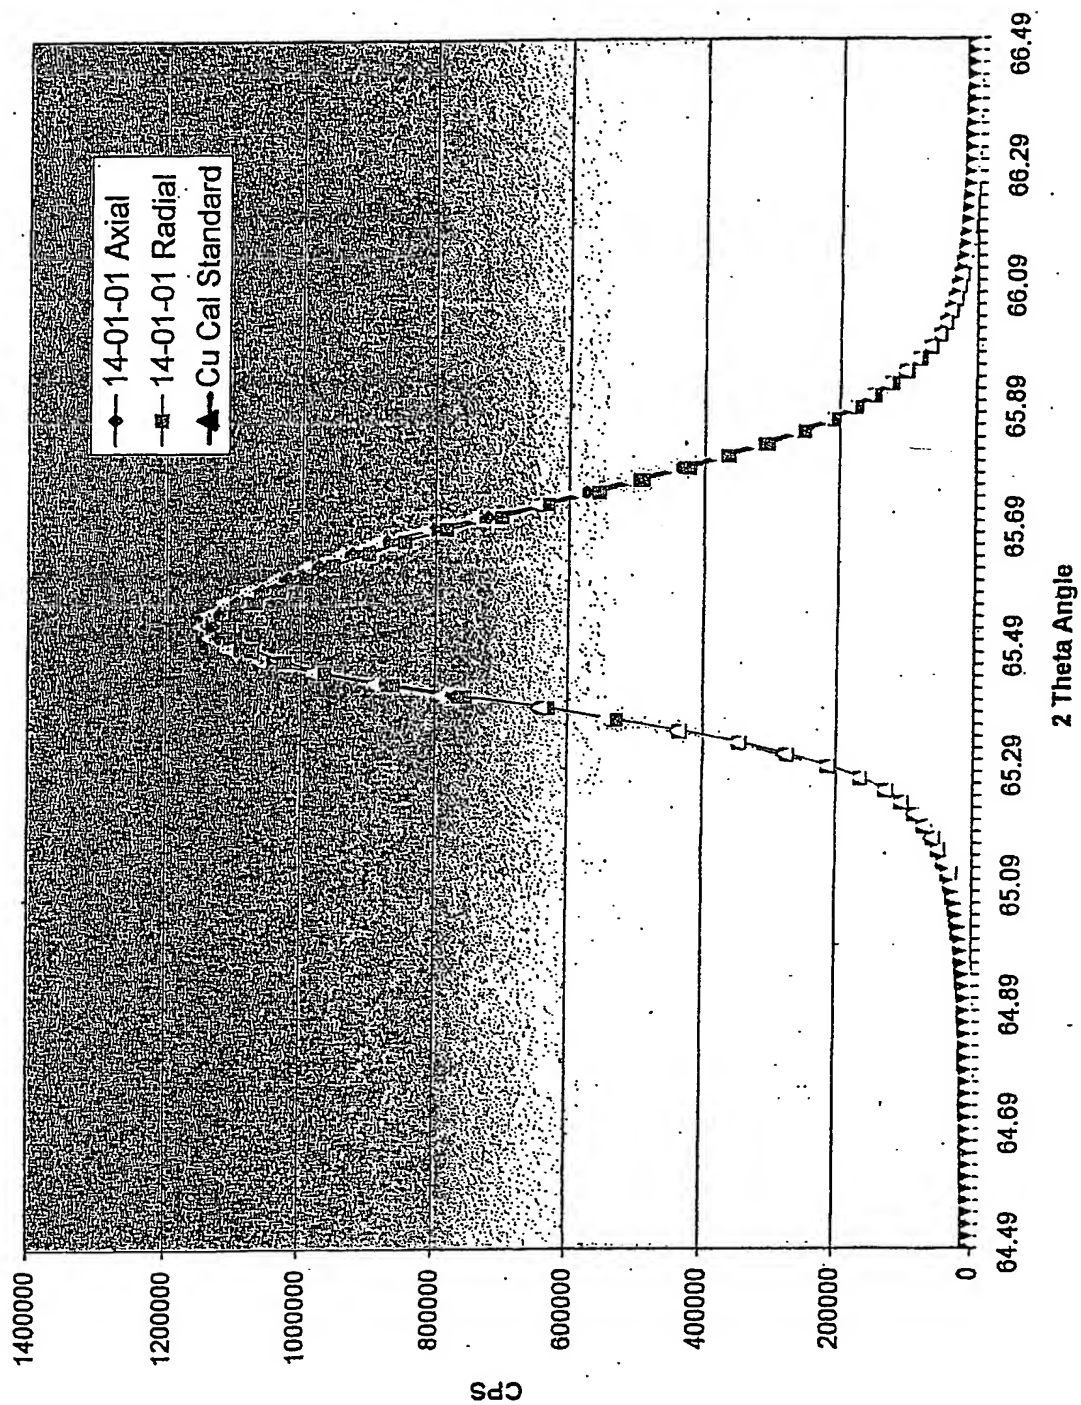


FIG. 25

Al in Copper 14-01-01


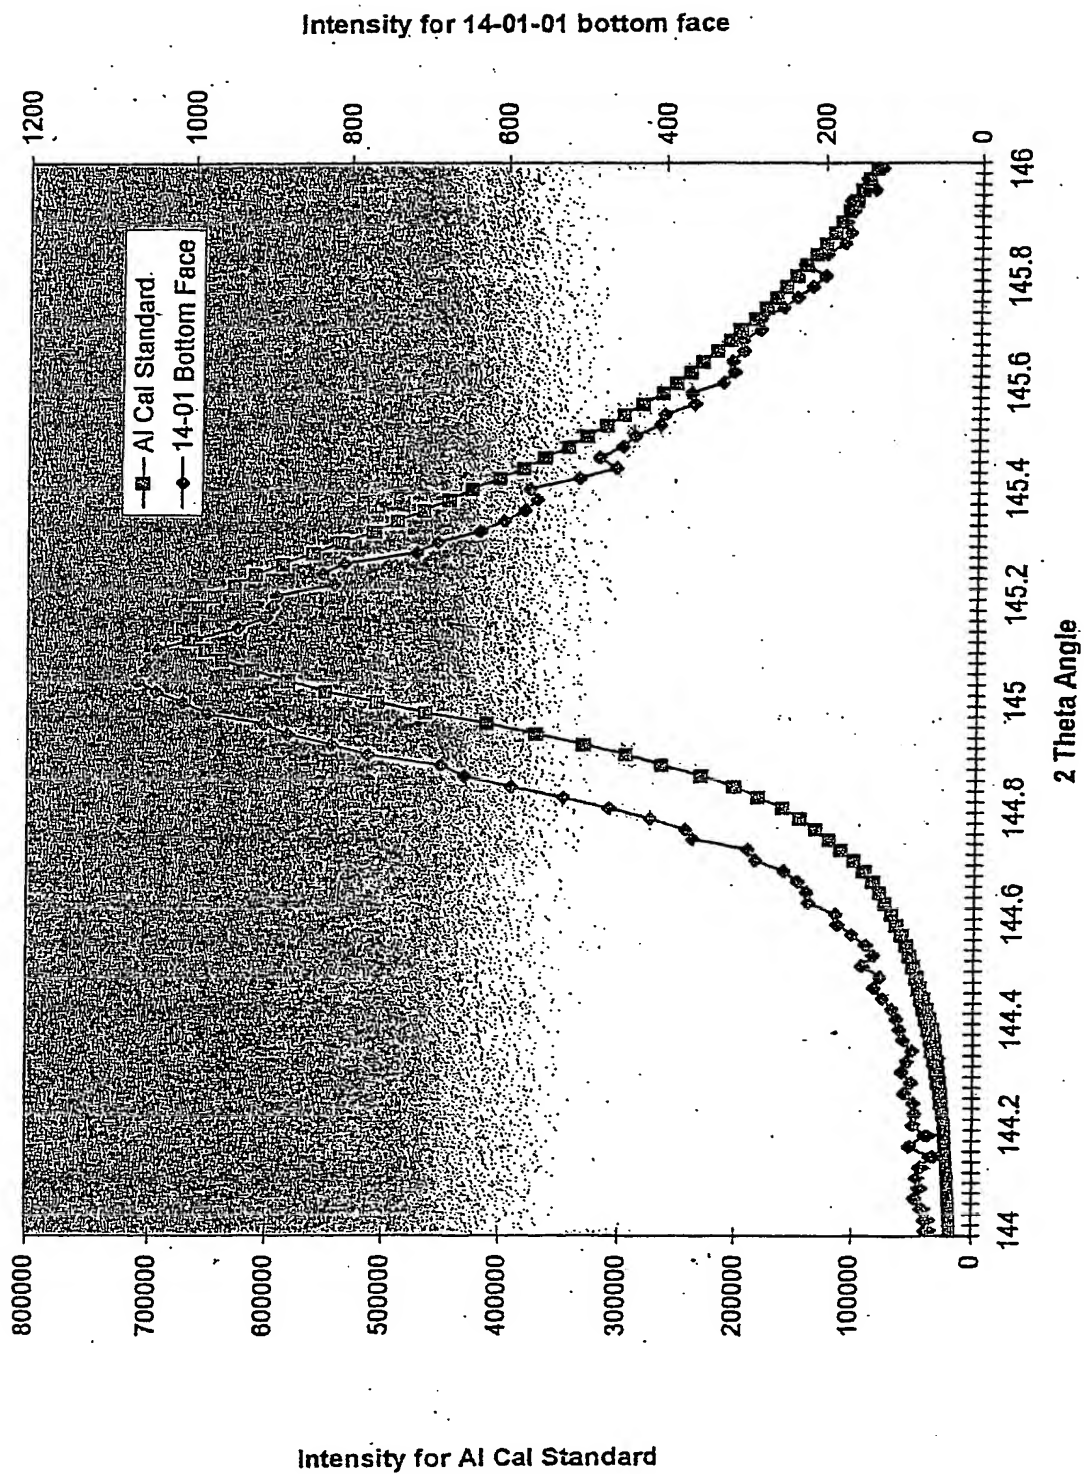


FIG. 26

Nickel Scans: Nickel Analysis

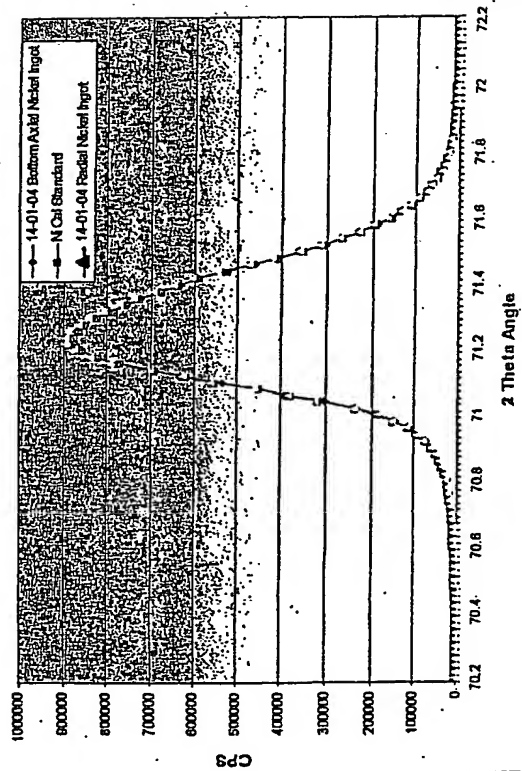

L α Nickel Scans
Run 14-01-04


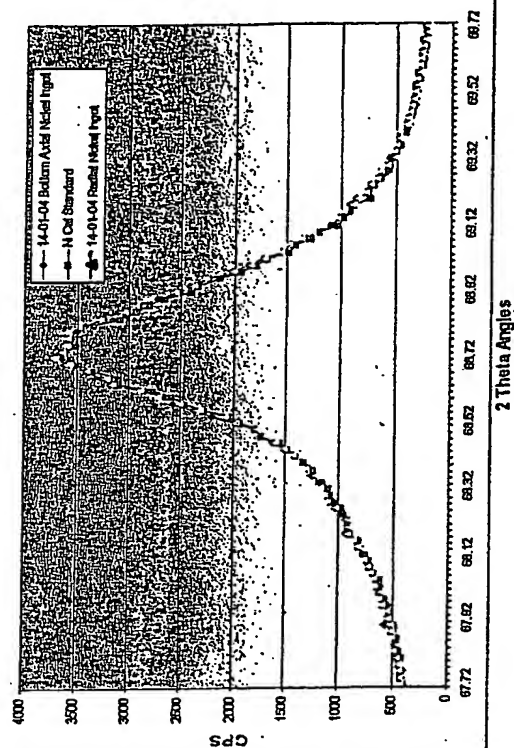


FIG. 27A

FIG. 27B

Nickel Scans: Al and Zr

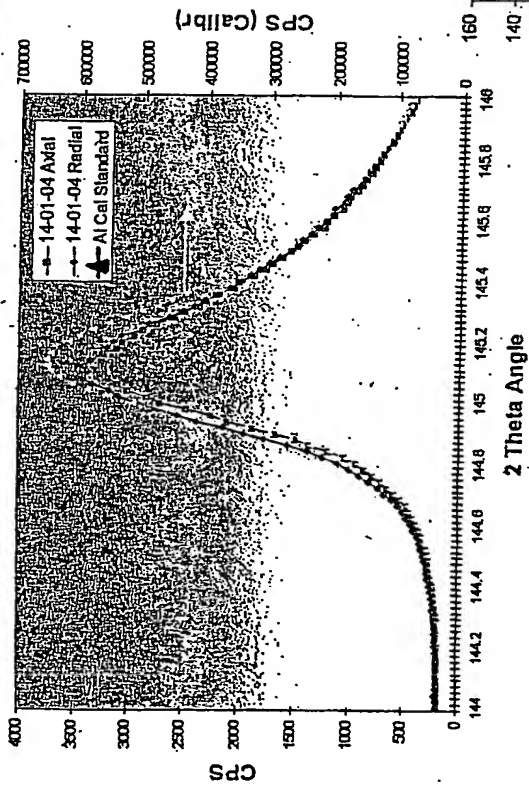

K_α Aluminum Scans of Nickel
Run 14-01-04

K_α Zirconium Scans of Nickel
Run 14-01-04

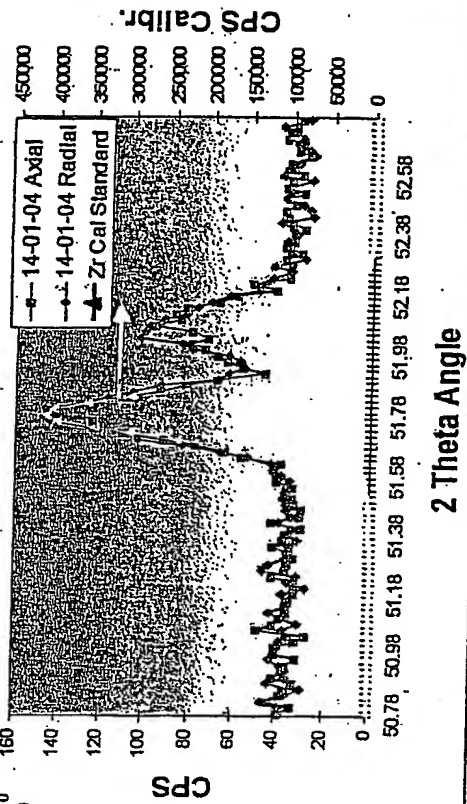



FIG. 28A

FIG. 28B

Nickel Scans: Sulfur on 6 sides

K_a Sulfur Scans of
Run 14-01-04

Nickel

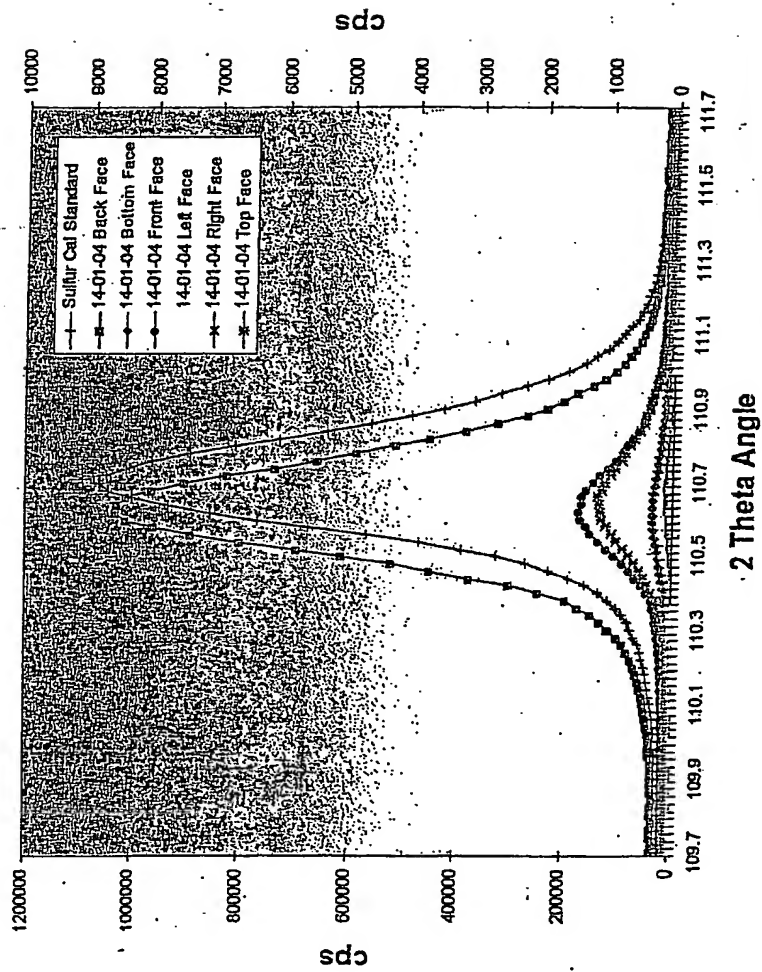

Ingot analyzed on
all six faces

FIG. 29

Nickel Scans: Cl

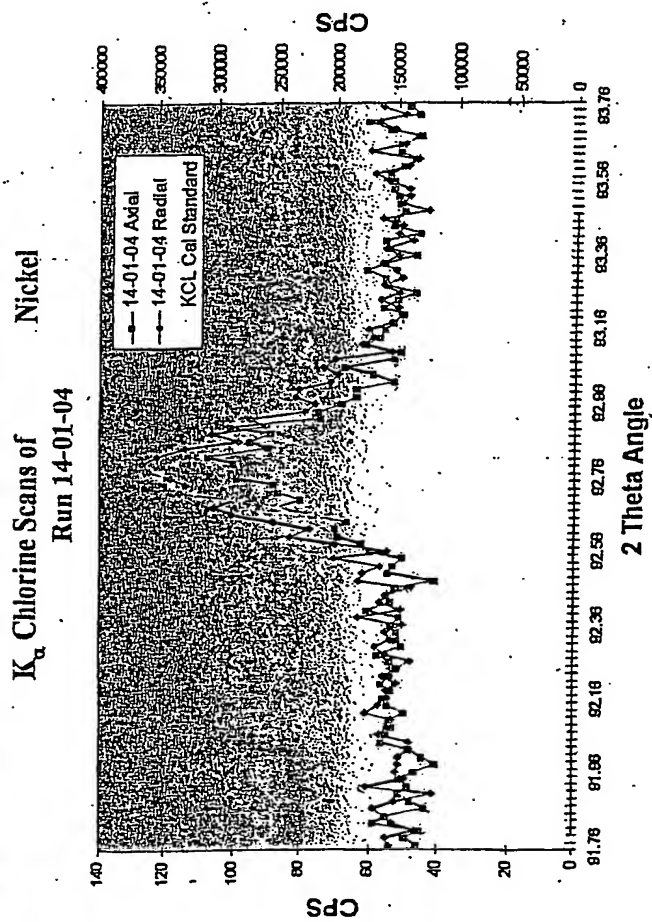


FIG. 30

Cobalt Scans: Cobalt Analysis

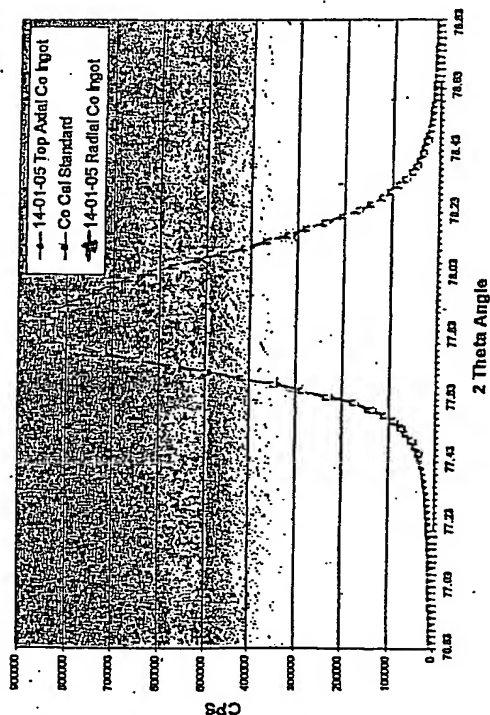


FIG. 31A

L_α Cobalt Scans
Run 14-01-05


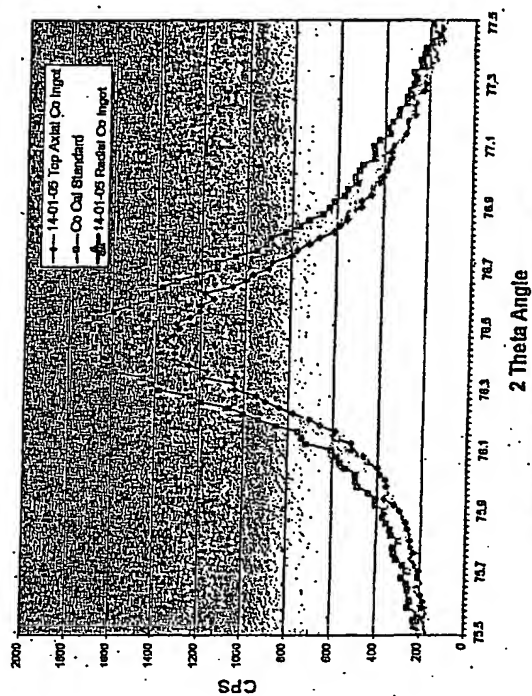


FIG. 31B

Cobalt Scans: Al and Fe

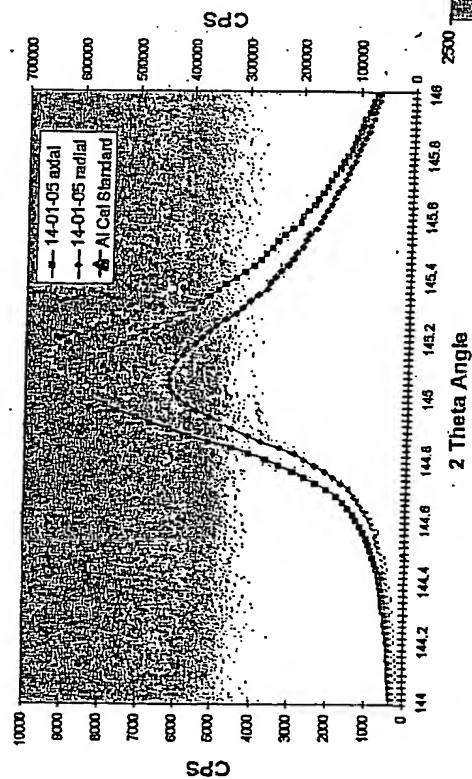

K_α Iron Scans of Cobalt


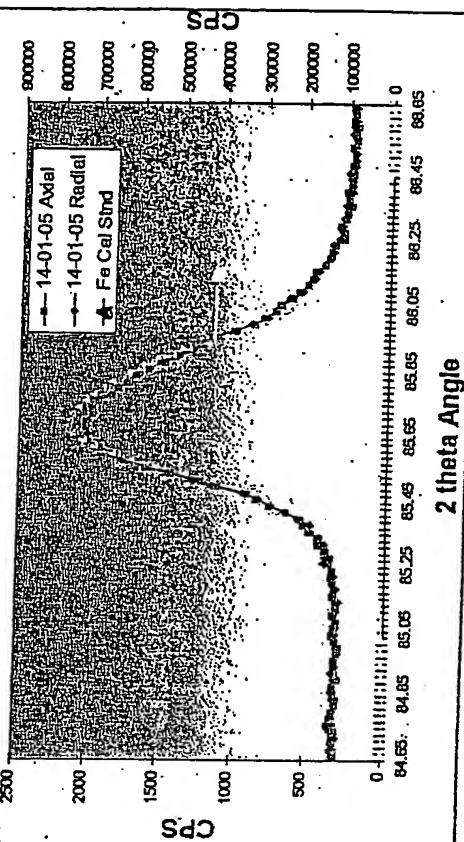



FIG. 32A

FIG. 32B

Cobalt Scans: Cl and Zr

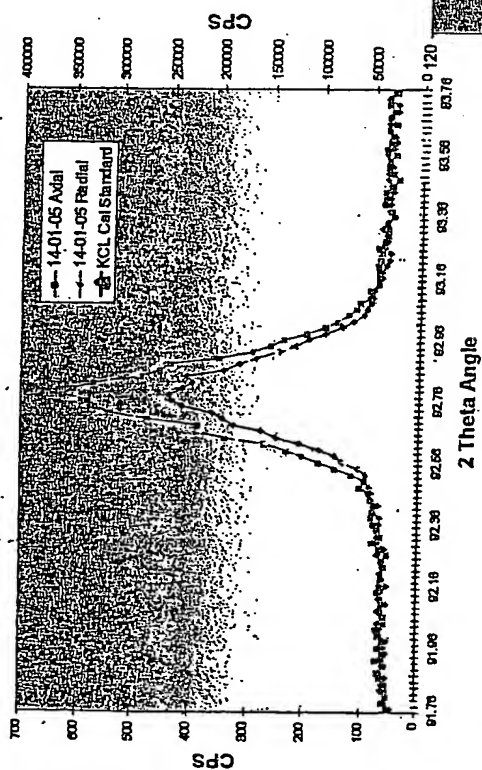

K_α Chlorine Scans of Cobalt
Run 14-01-05

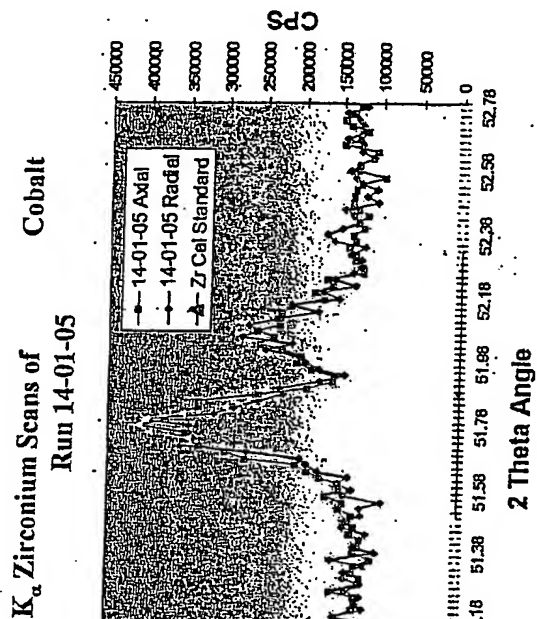


K_α Zirconium Scans of Cobalt
Run 14-01-05

FIG. 33A

FIG. 33B

Cobalt Scans: Mn

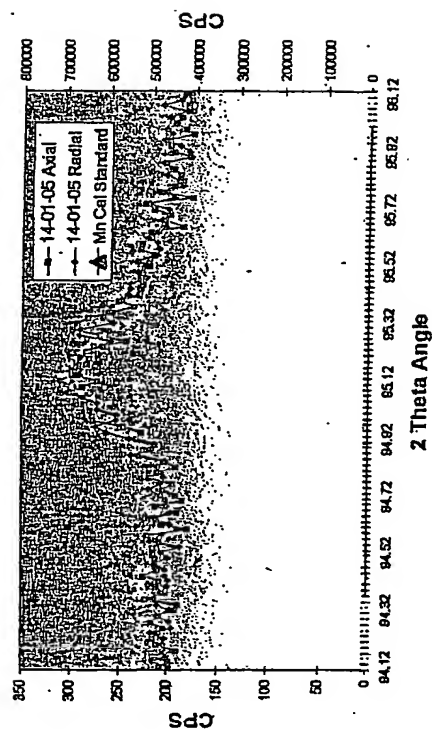

K_a Manganese Scans of
Run 14-01-05

Cobalt

FIG. 34

14-01-06 Cu - Axial and Radial Samples vs Cu Cal Standard (LiF200/FPC)

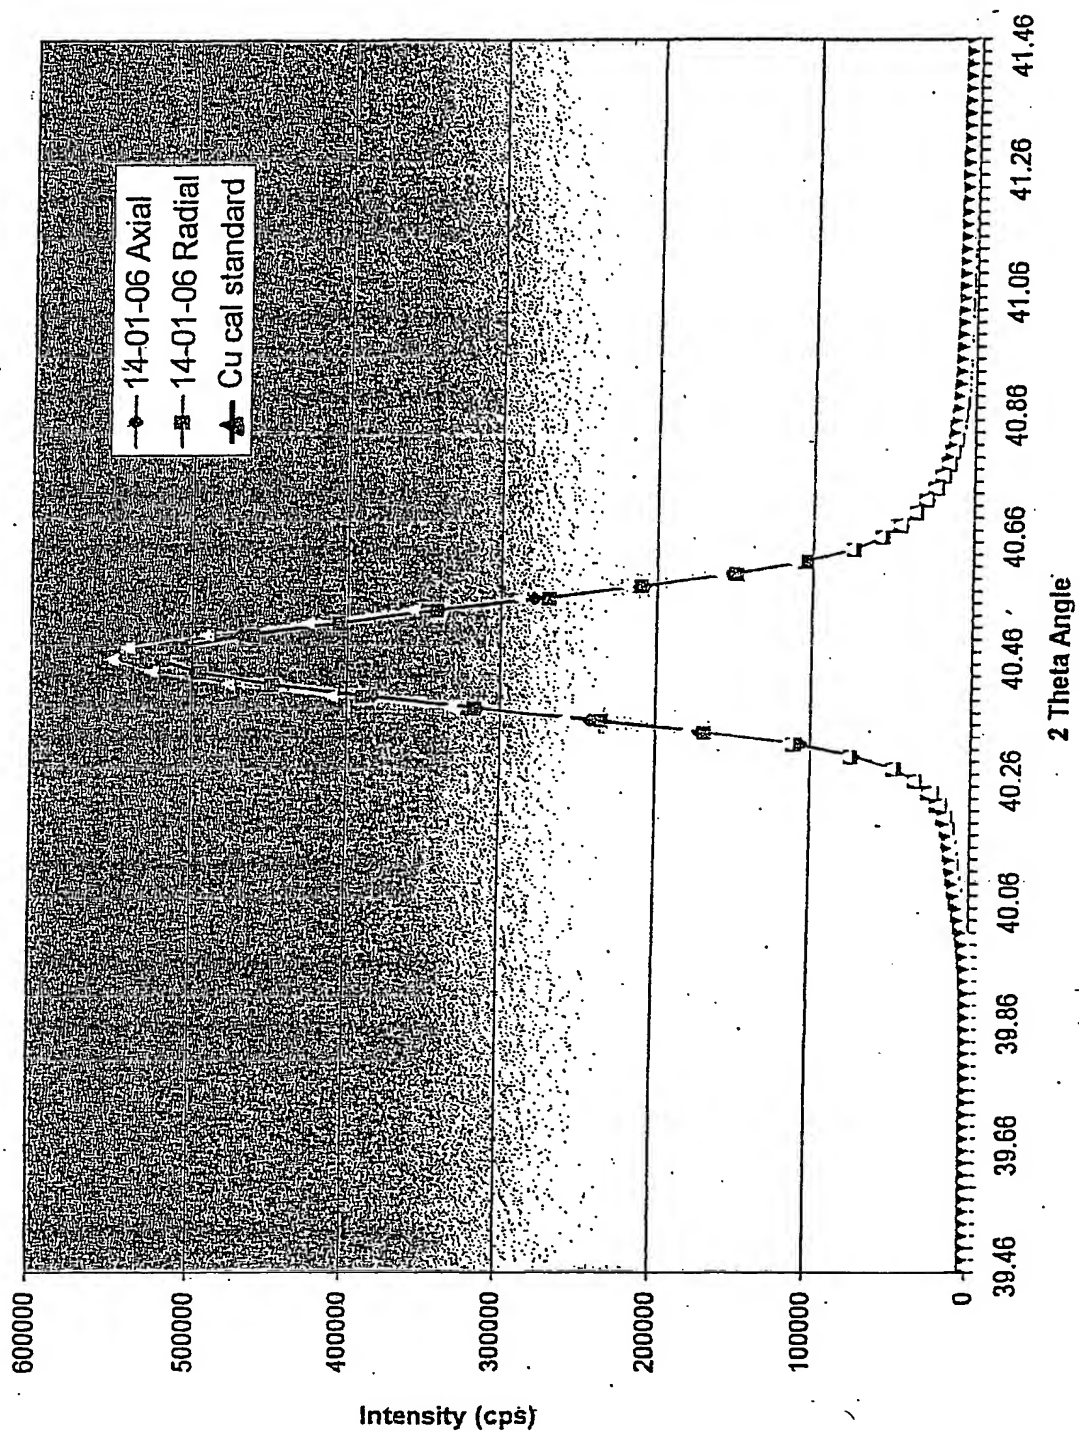


FIG. 35

14-01-06 Au- Axial and Radial Samples vs Au Cal Standard (LiF420/SC)

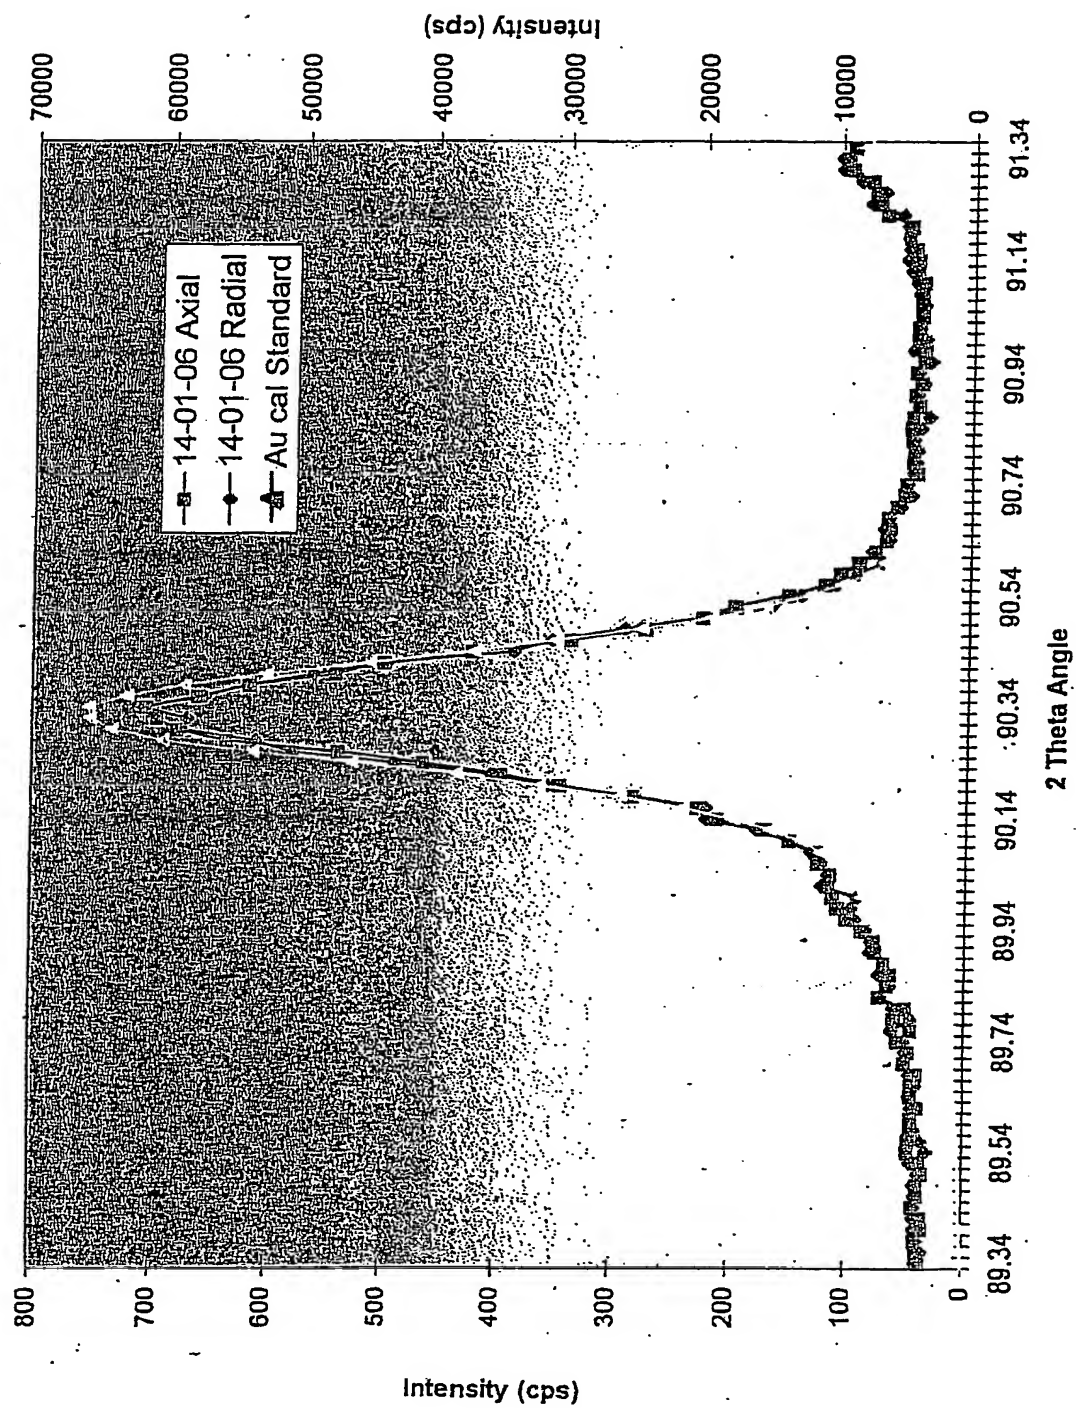


FIG. 36

14-01-06 Ag: Axial and Radial Samples vs Ag Cal Standard (LiF220/SC)

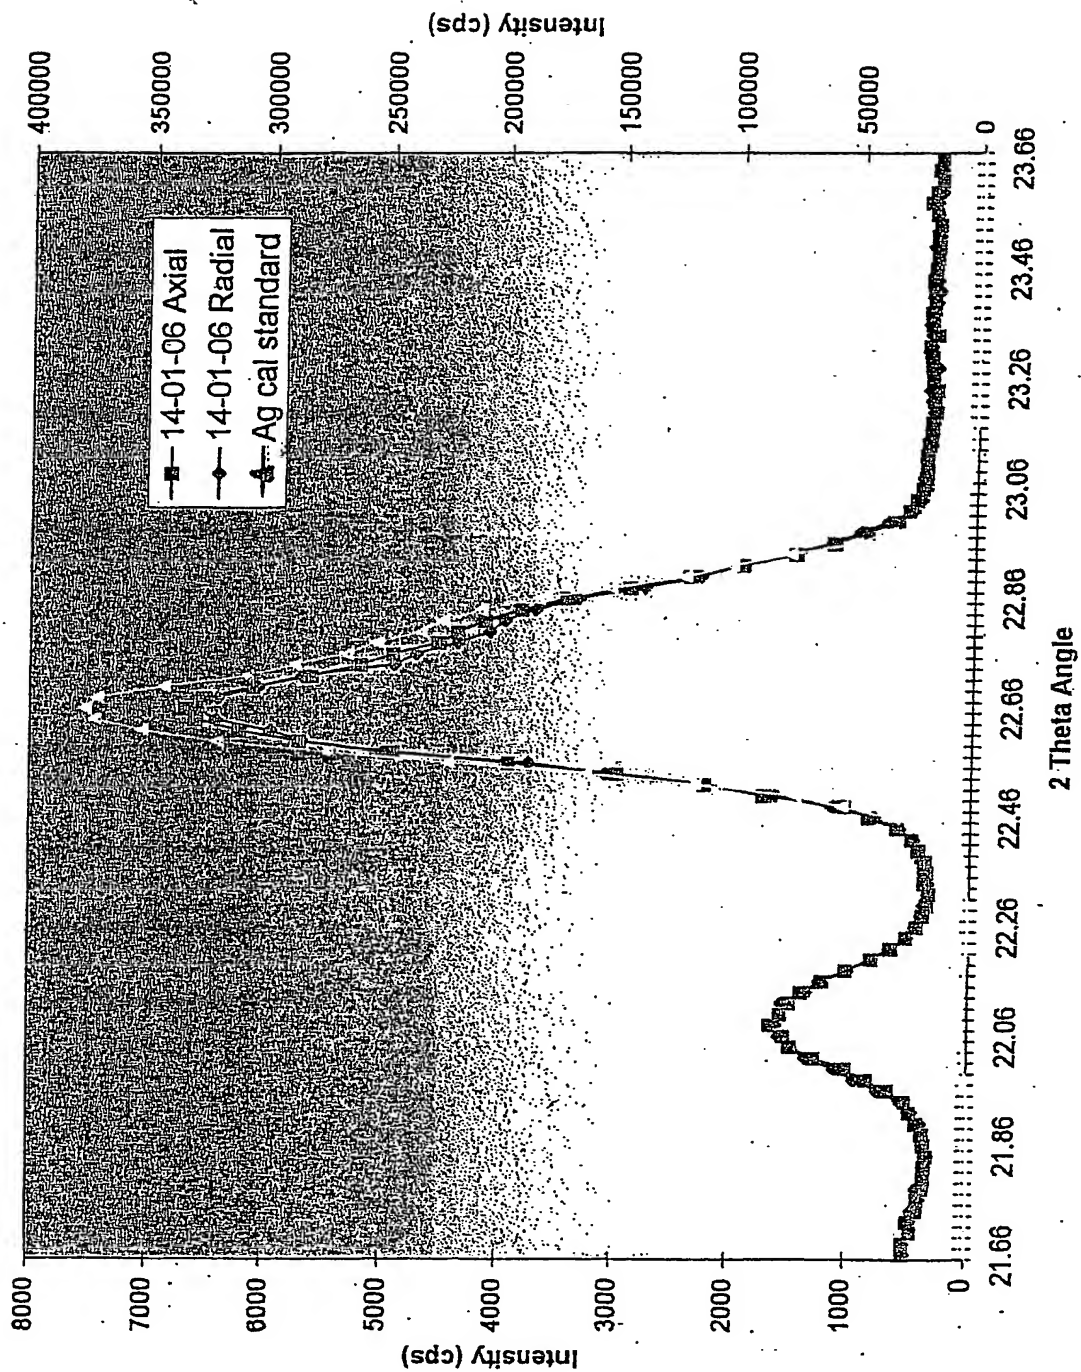


FIG. 37

14-01-07 Sn- Axial and Radial vs Sn Cal Standard

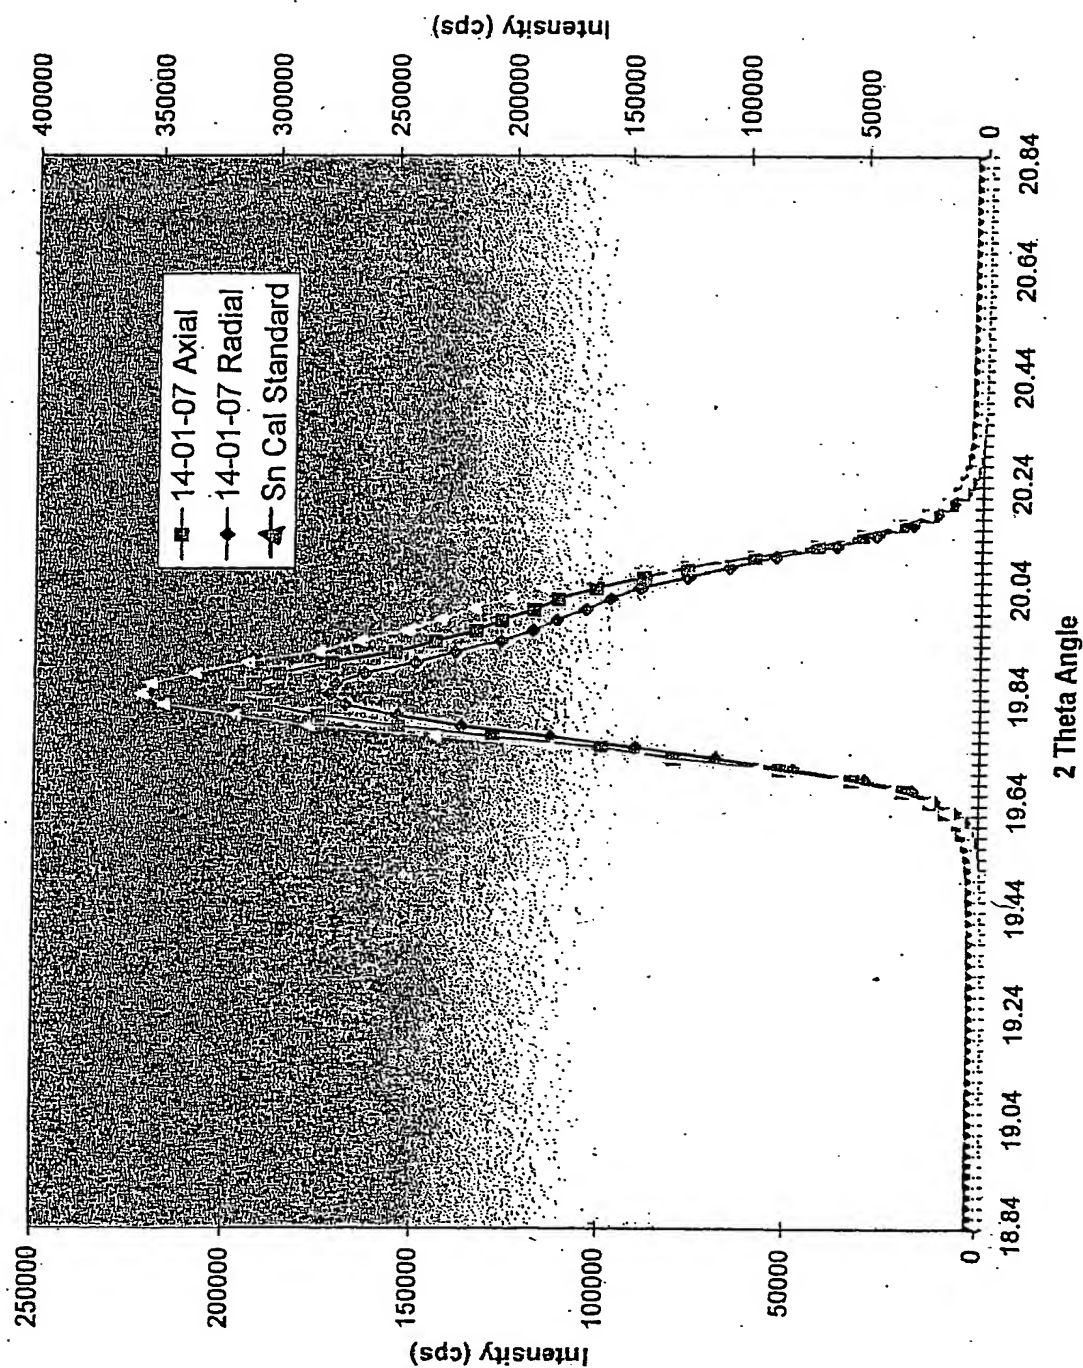


FIG. 38

14-01-07 Zn-- Axial and Radial vs Zn Cal Standard (LIF220/FPC)

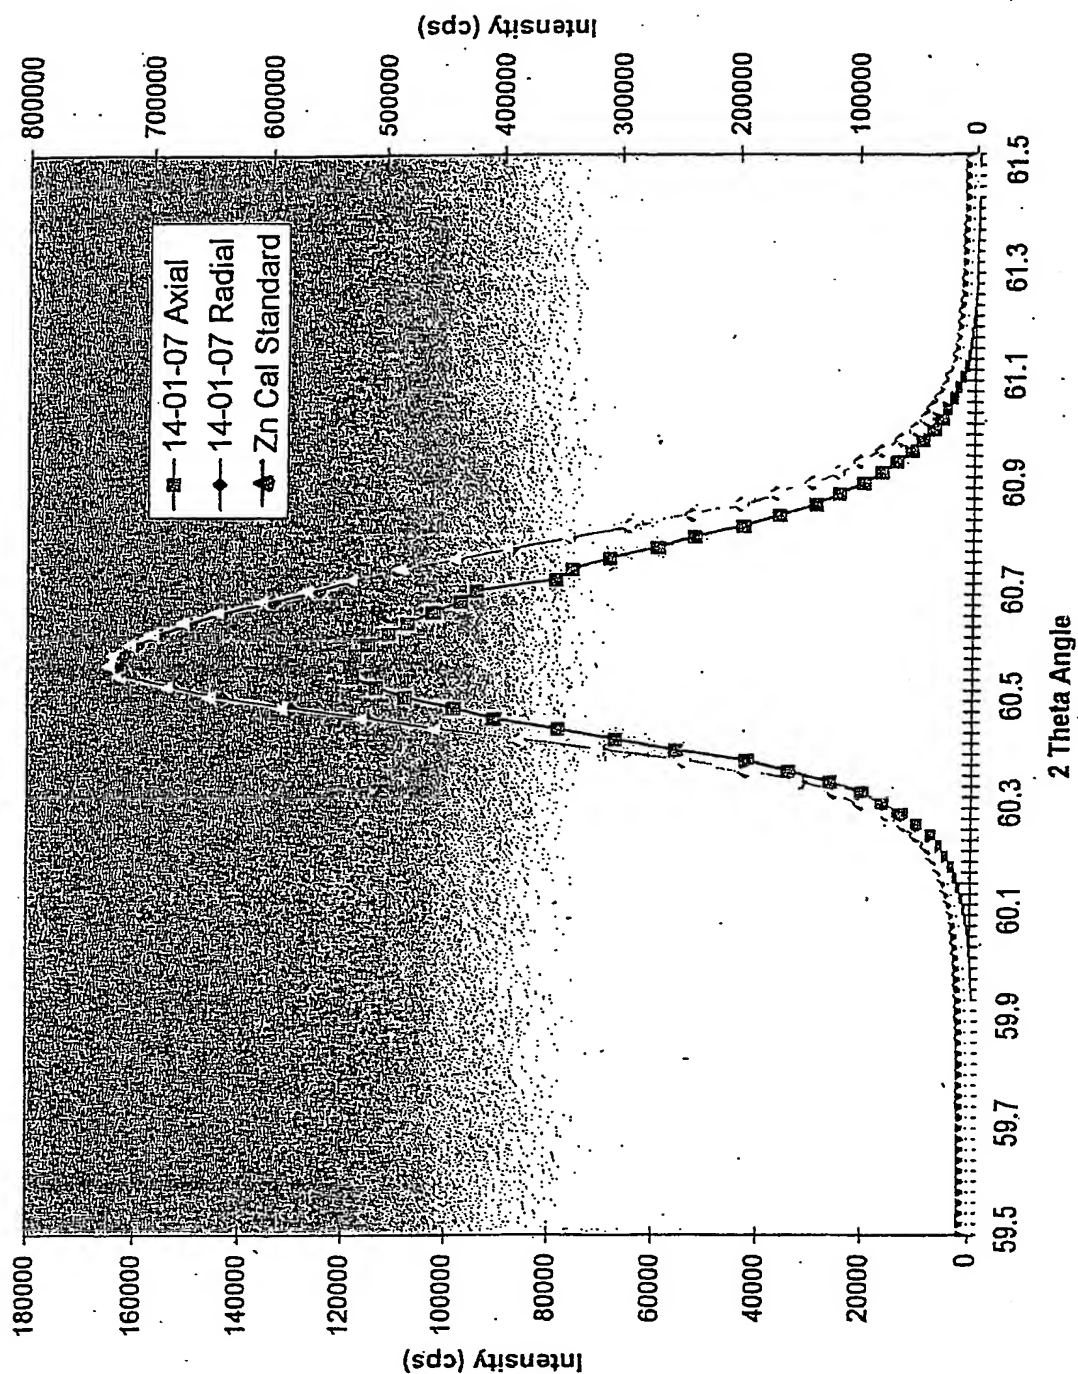


FIG. 39

14-01-07 Pb- Axial and Radial vs Pb Cal Standard

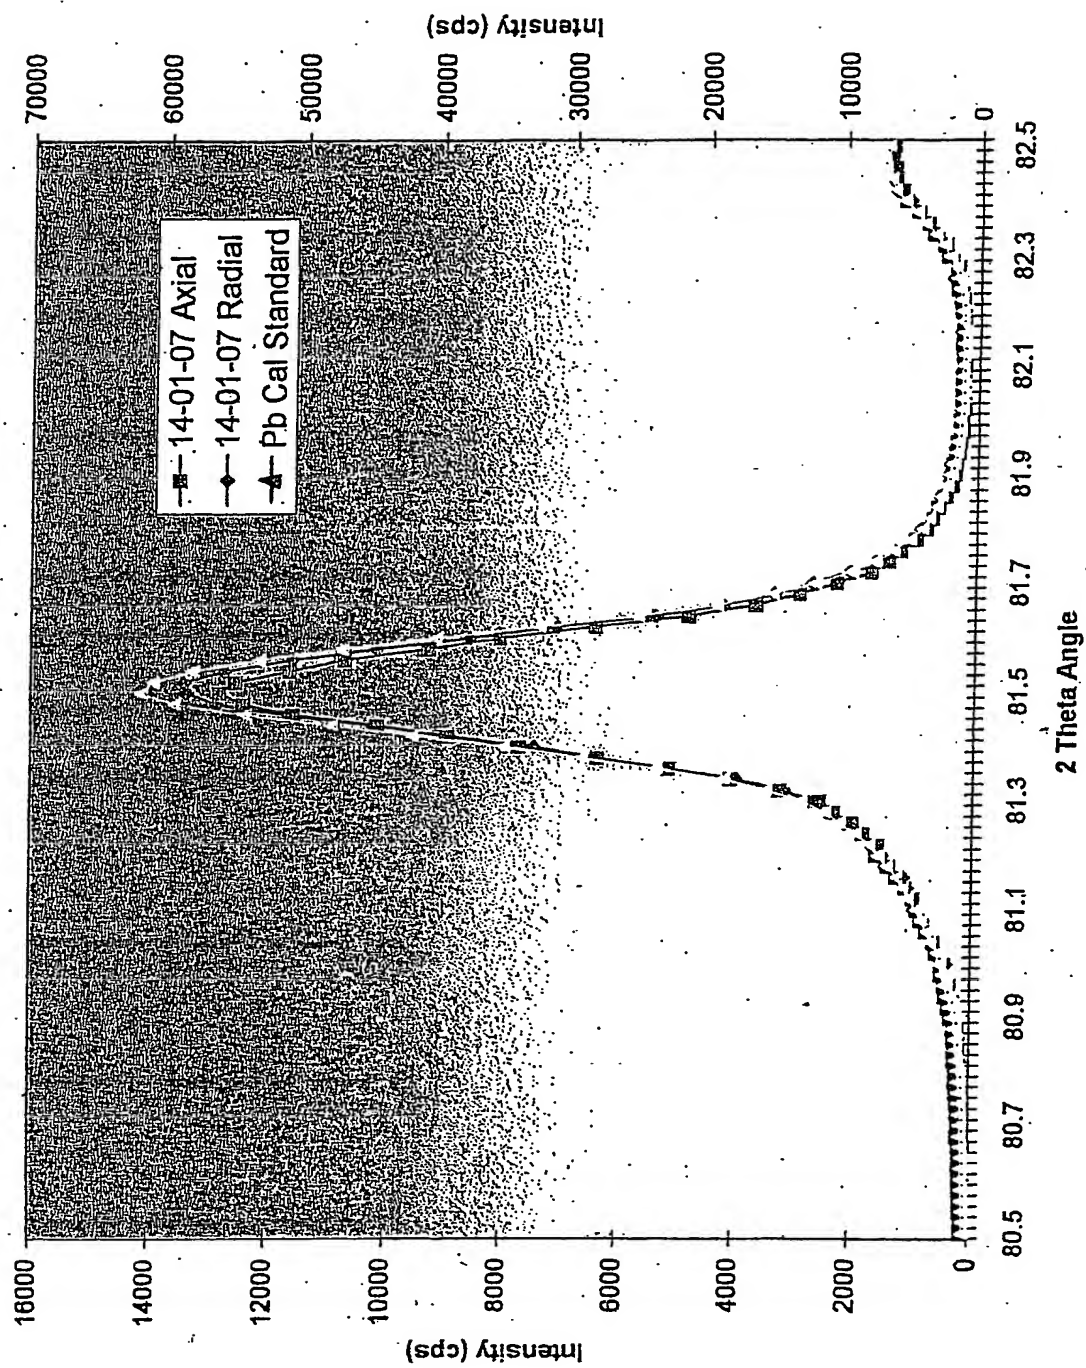


FIG. 40

14-01-08 scans for K

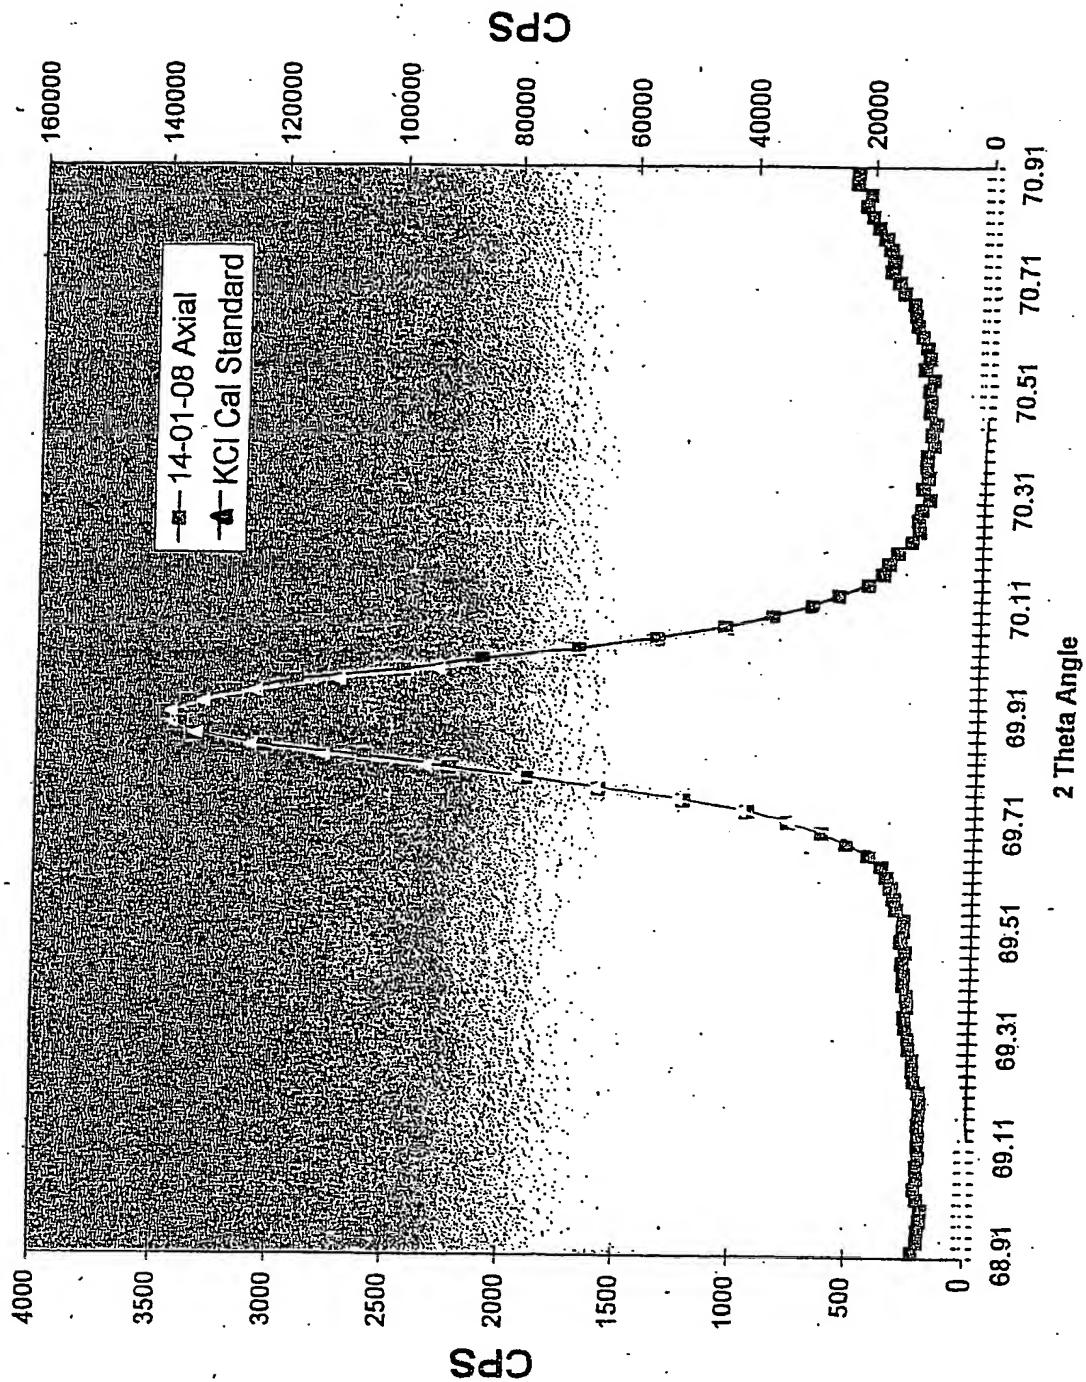


FIG. 41

14-01-08 Sn- Axial and Radial vs Sn Cal Standard

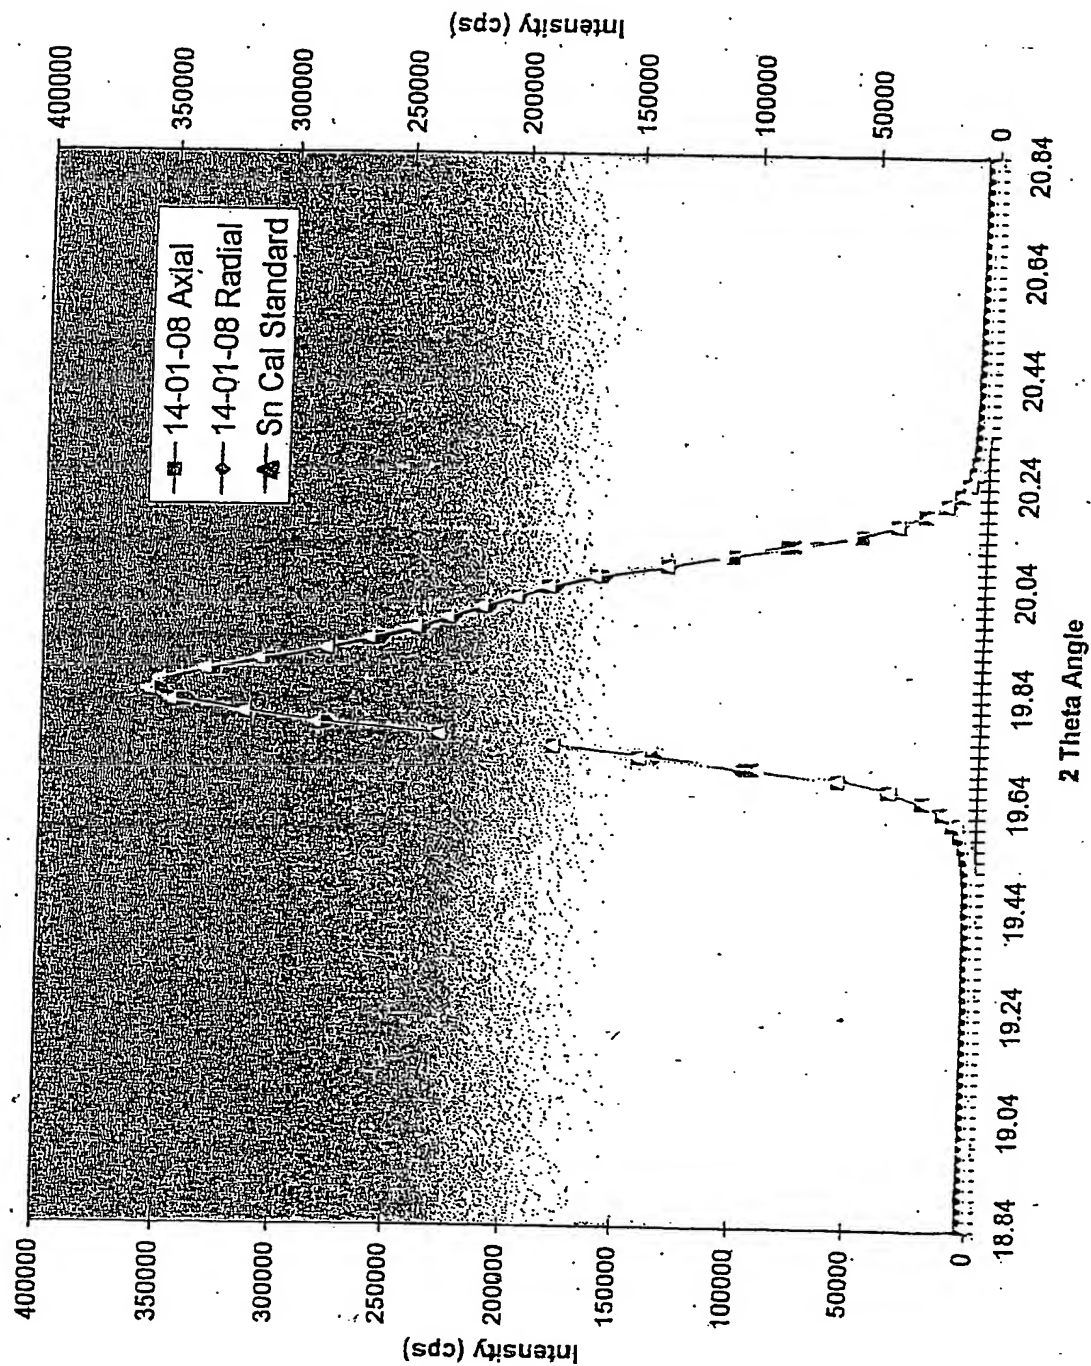


FIG. 42

14-01-08 Mg- Axial and Radial Samples vs MgO Cal Standard

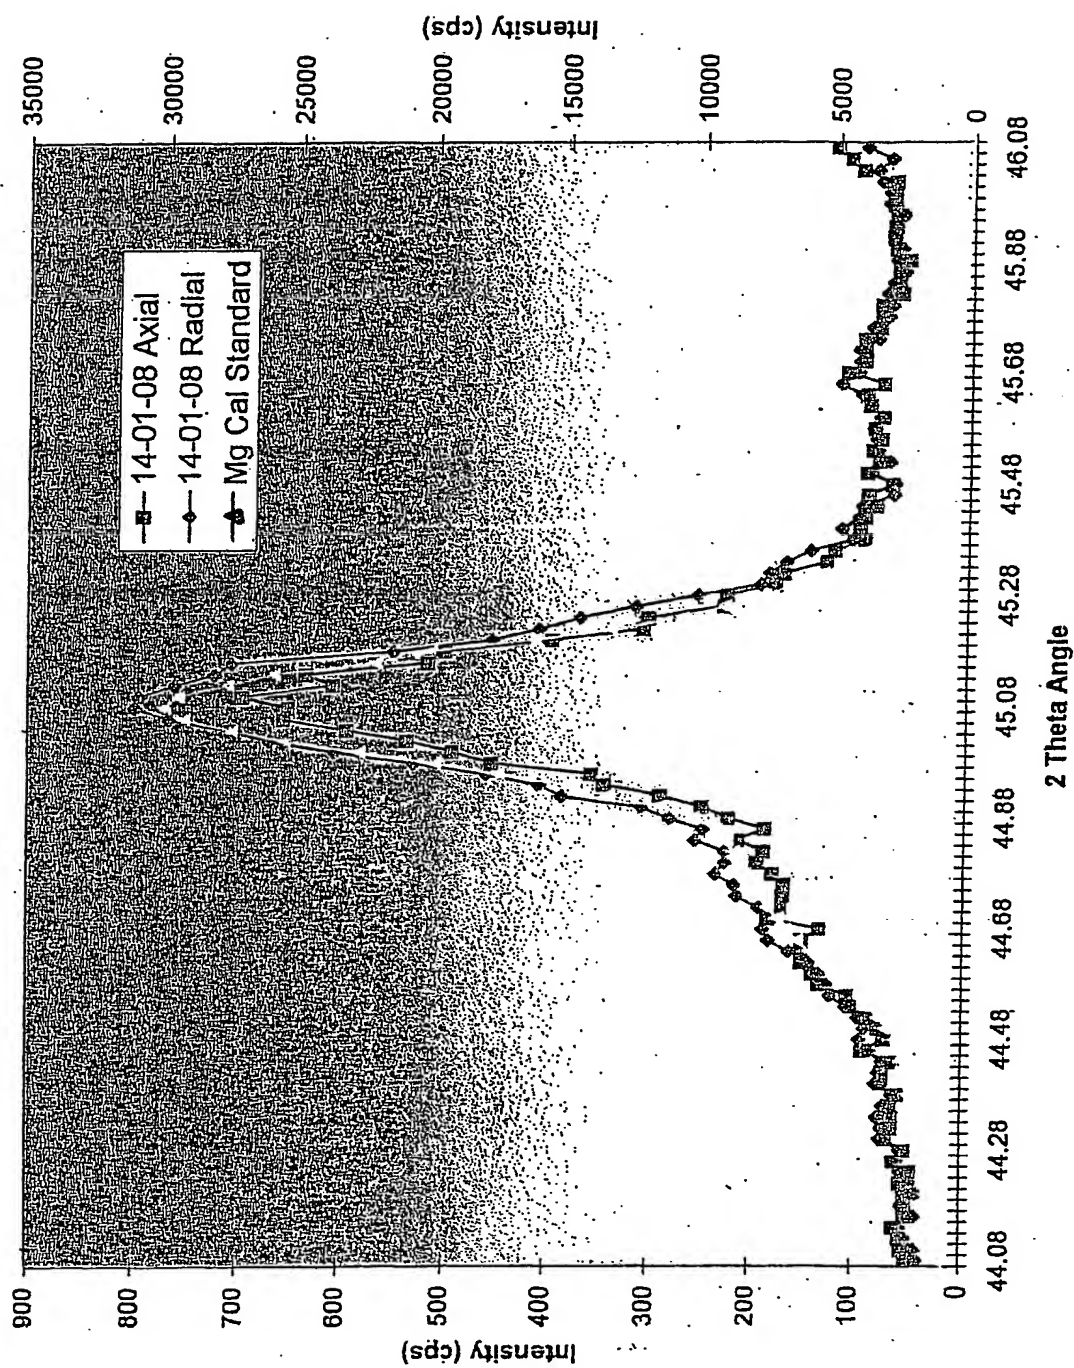


FIG. 43

14-01-08 Na- Axial and Radial Samples vs AlNa3F6 Cal Standard


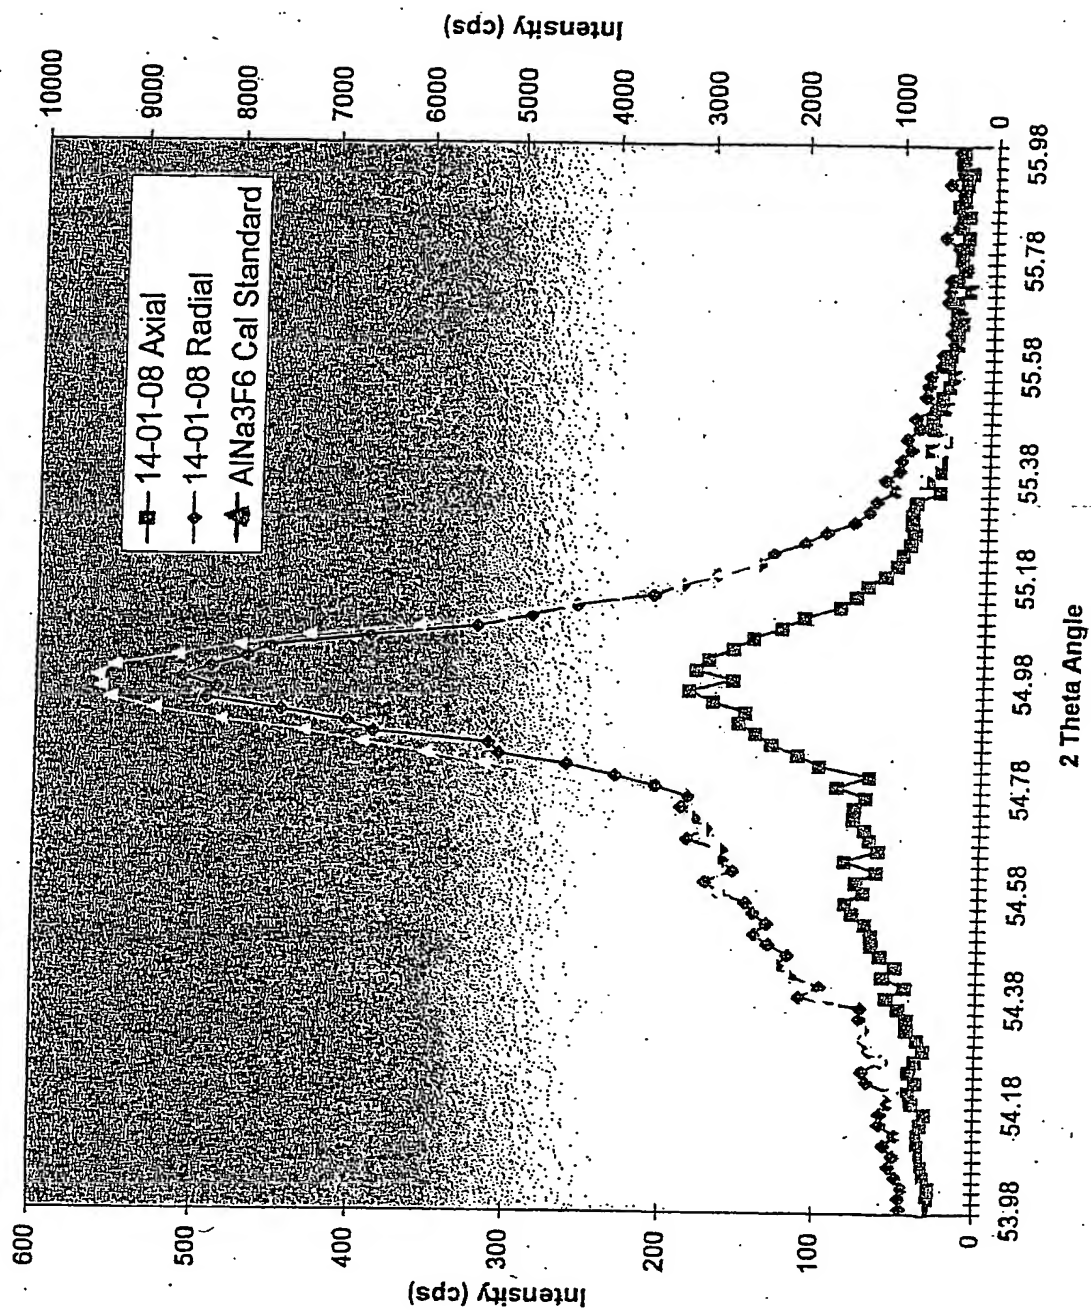


FIG. 44

Silicon Scans: Silicon Analysis

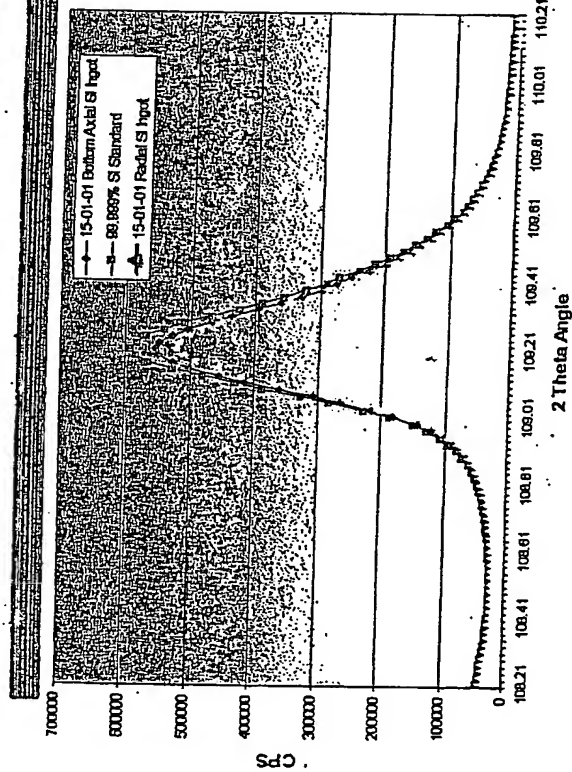

L ρ Silicon Scans
Run 15-01-01


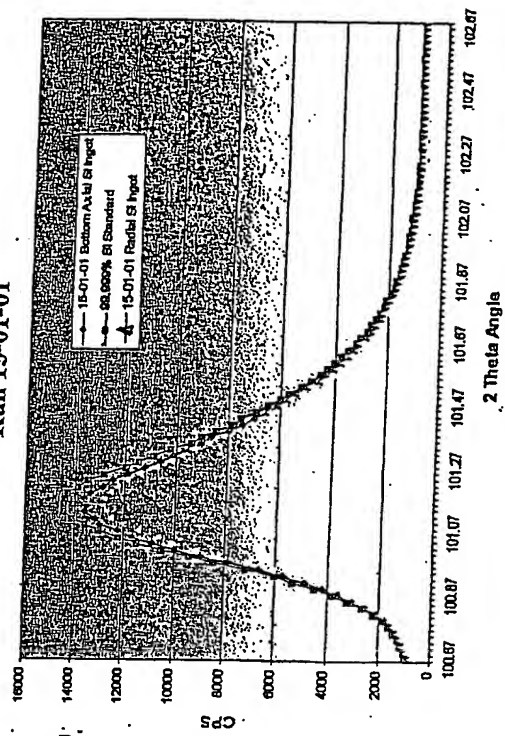


FIG. 45B

FIG. 45A

Silicon Scans: Al and Ti

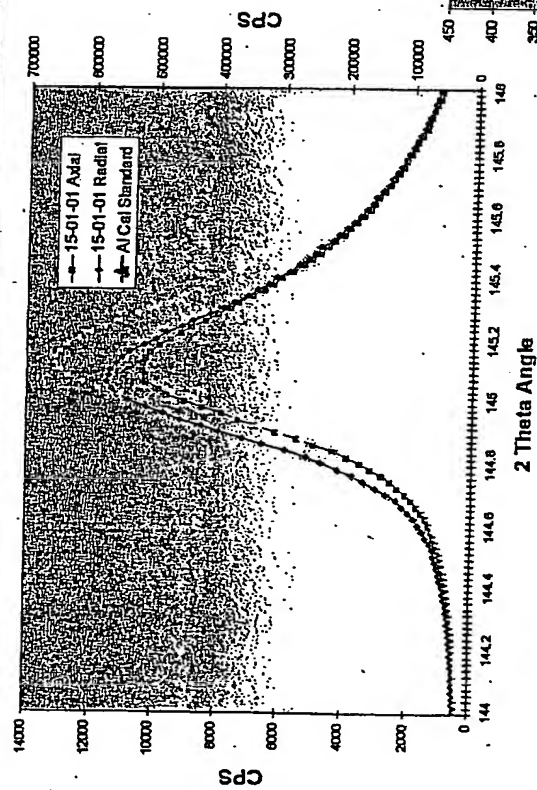

K_α Titanium Scans of Silicon


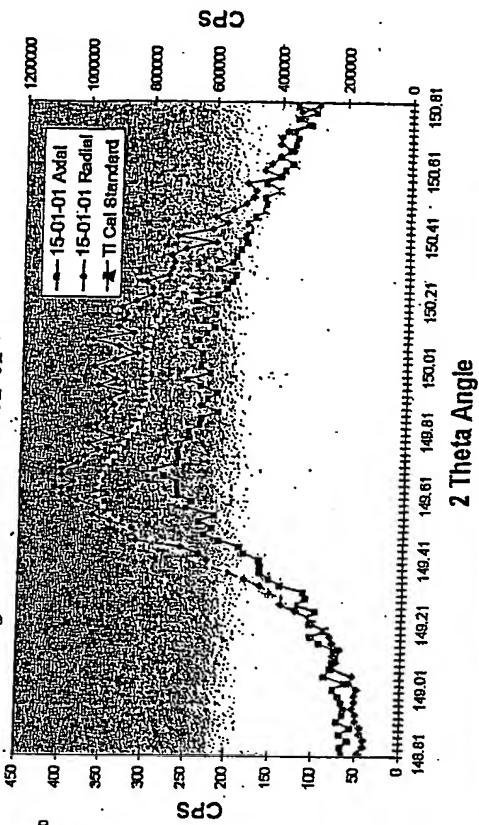


FIG. 46A

FIG. 46B

Silicon Scans: S and Cl

K_α Sulfur Scans of Silicon
Run 15-01-01

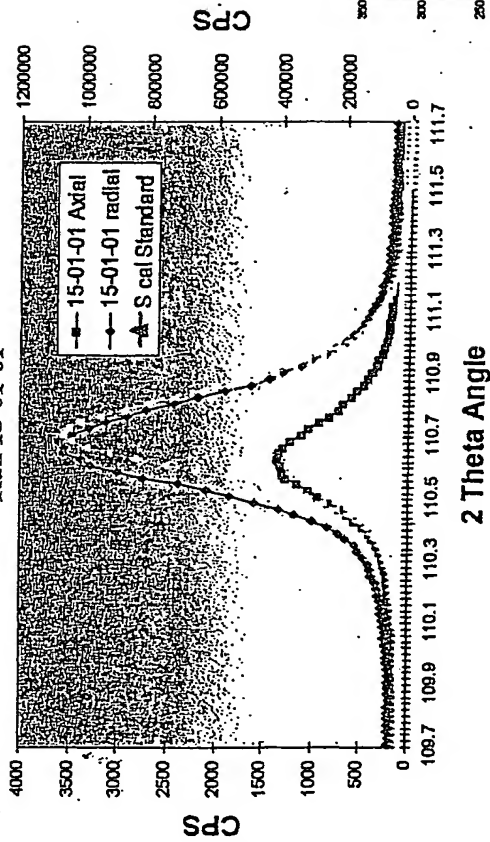

K_α Chlorine Scans of Silicon
Run 15-01-01


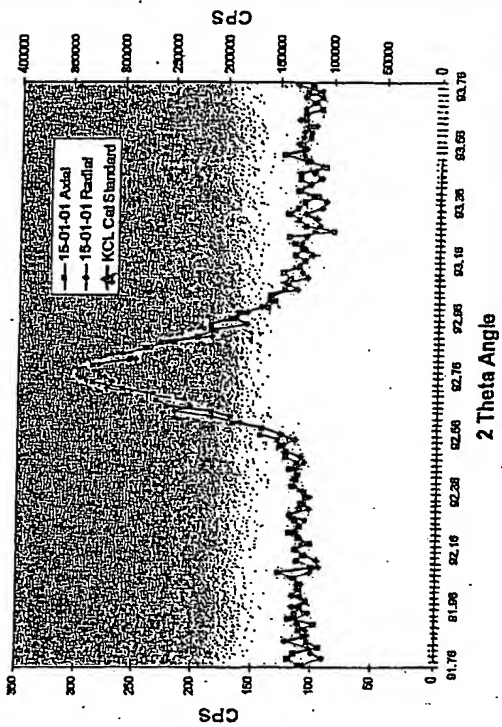


FIG. 47A

FIG. 47B

Silicon Scans: Ga and K

K_{α} Gallium Scans of Silicon
Run 15-01-01

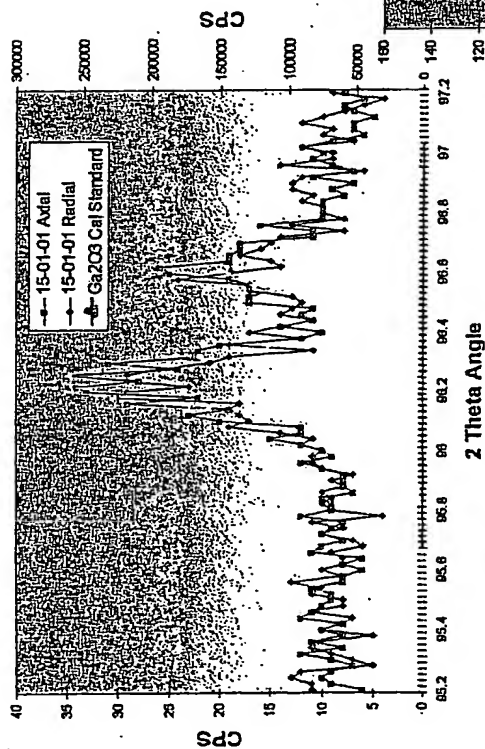

K_{α} Potassium Scans of Silicon
Run 15-01-01


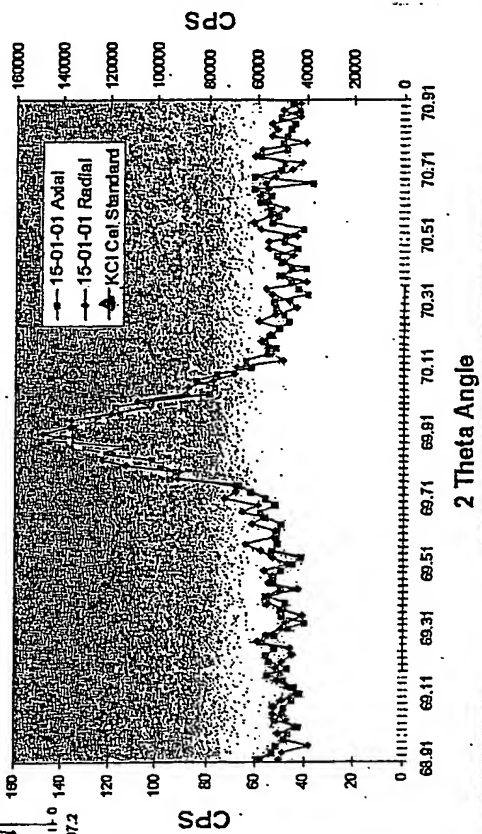


FIG. 48B

FIG. 48A

Iron Scans: Iron Analysis

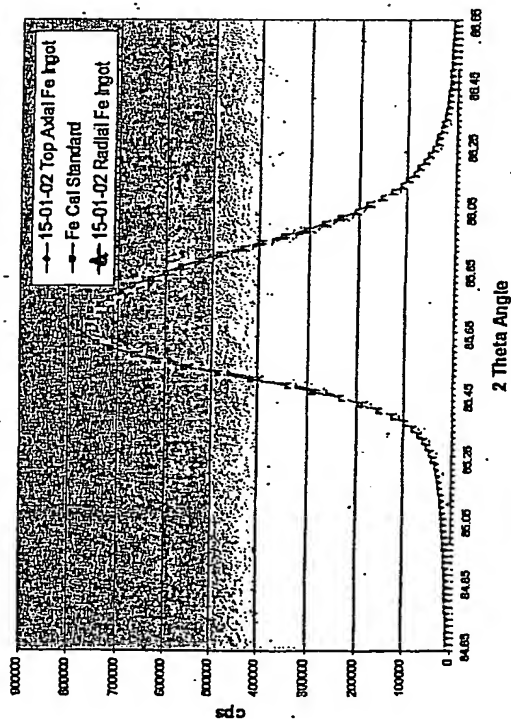

K_α Iron Scans of Iron
Run 15-01-02

L_α Iron Scans of Iron
Run 15-01-02


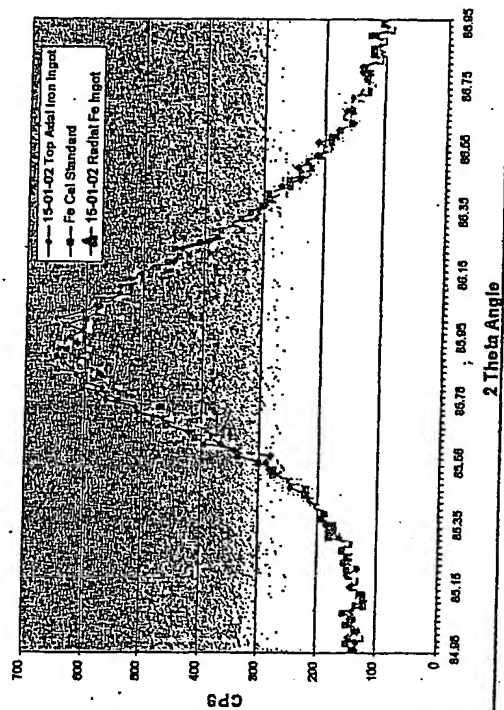


FIG. 49A

FIG. 49B

Iron Scans: Al and Zr

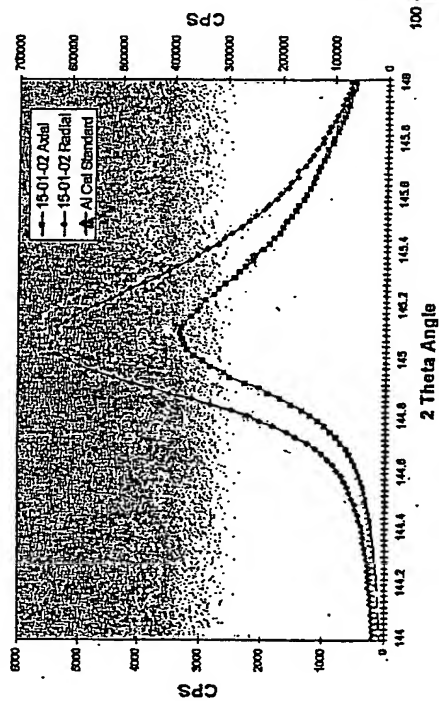

K_α Zr Scans of Iron

Run 15-01-02


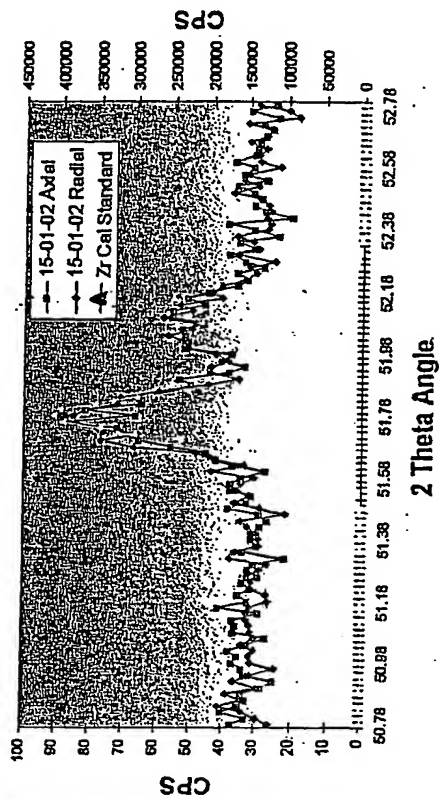


FIG. 50A

FIG. 50B

Iron Scans: S and Cl

K_{α} Sulfur Scans of Iron
Run 15-01-02

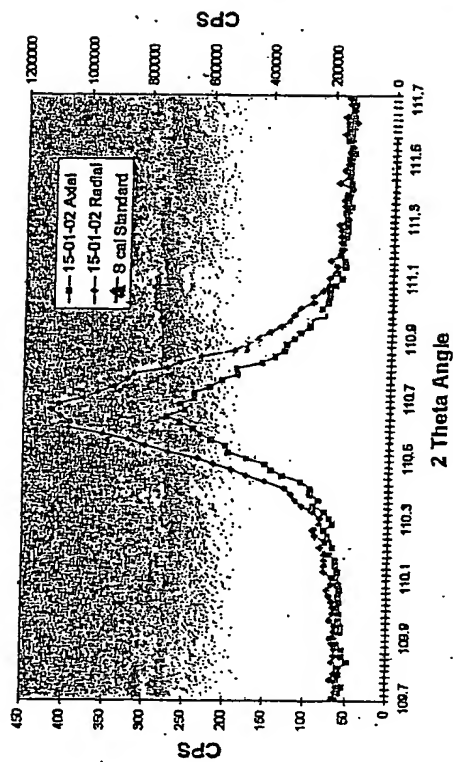

K_{α} Chlorine Scans of Iron
Run 15-01-02

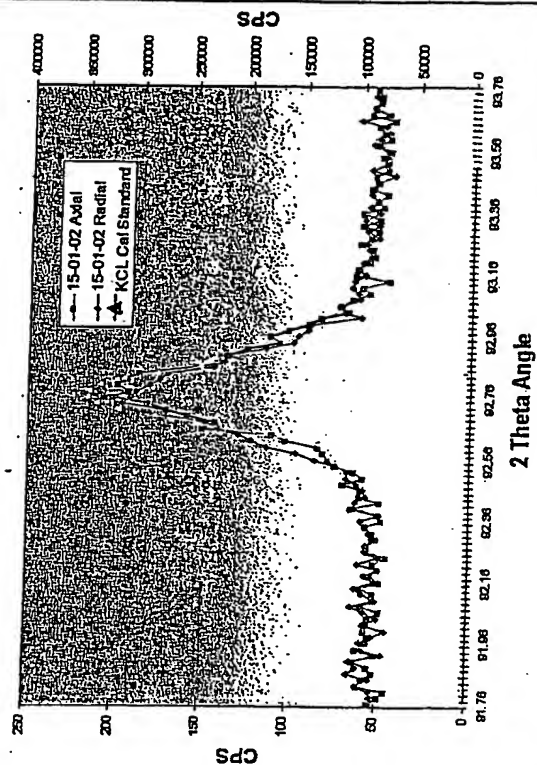


FIG. 51B

FIG. 51A

15-01-03 Cr- Axial and Radial Samples vs Cr2O3 Cal Standard (LiF220/FPC)

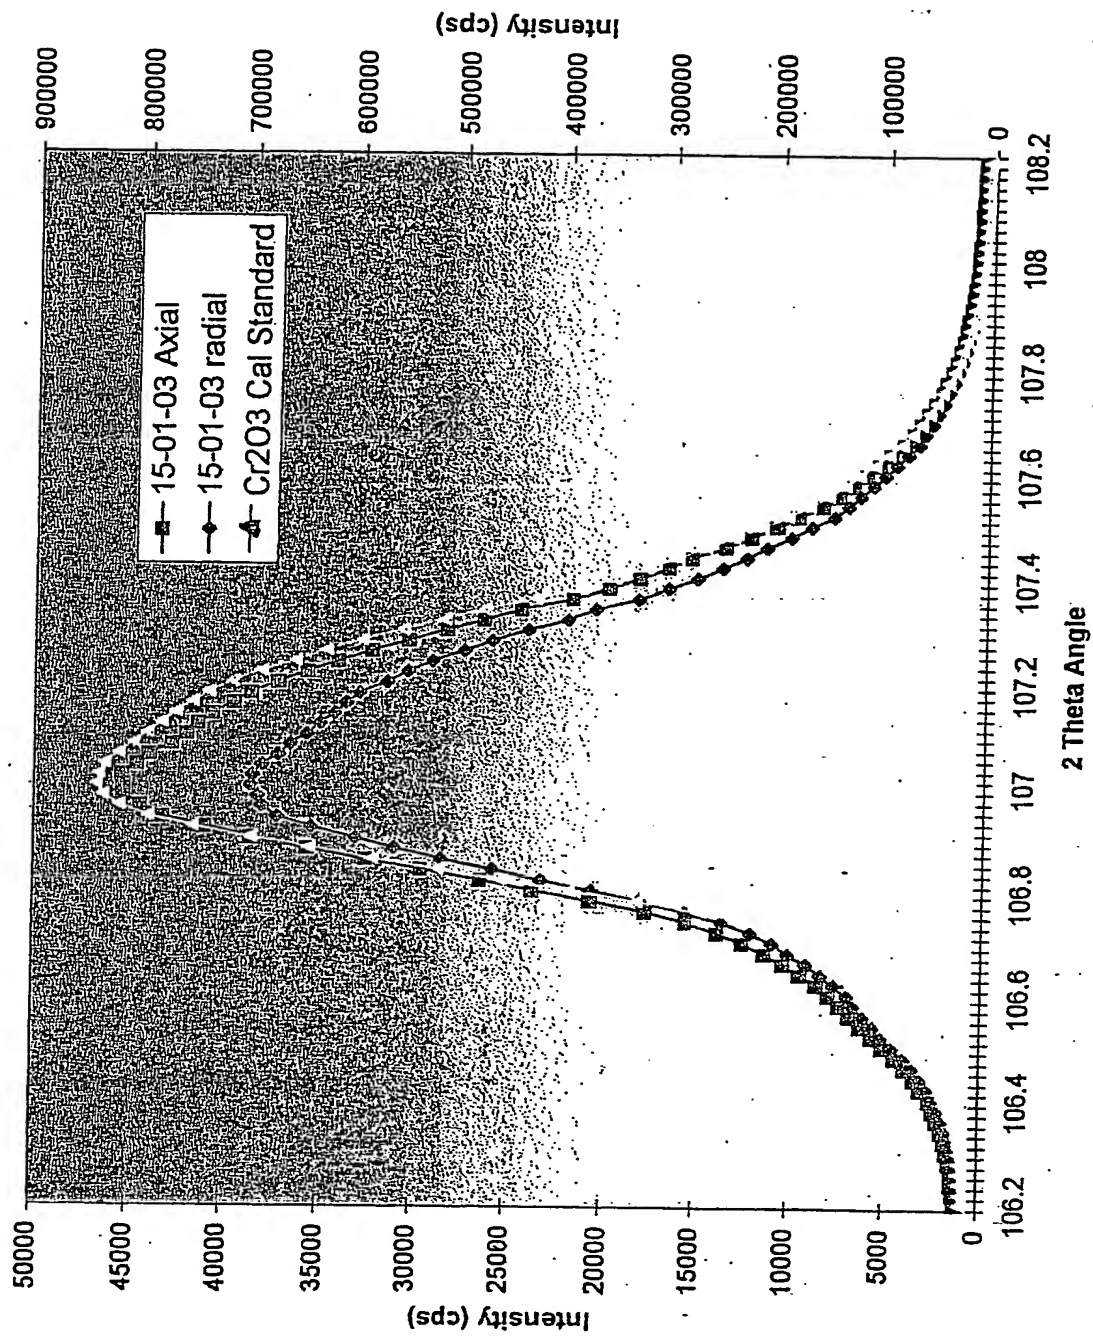


FIG. 52

15-01-03 Fe- Axial and Radial vs Fe Cal Standard (LiF220/FPC)

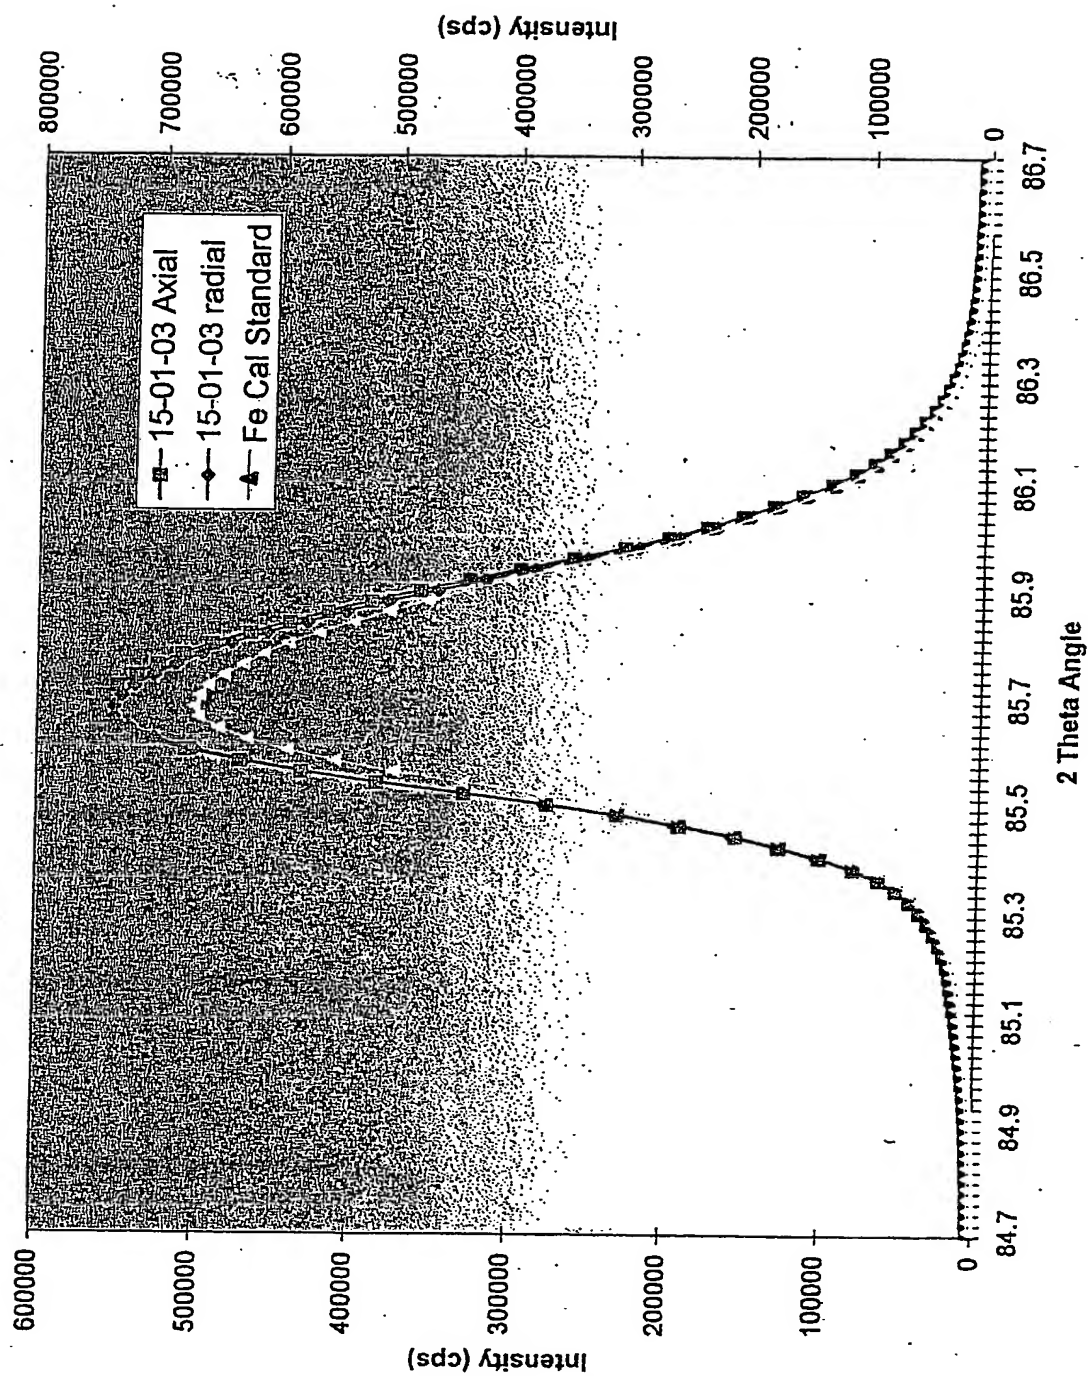


FIG. 53

15-01-03 V- axial and radial samples vs V cal standard (LiF220/FPC)

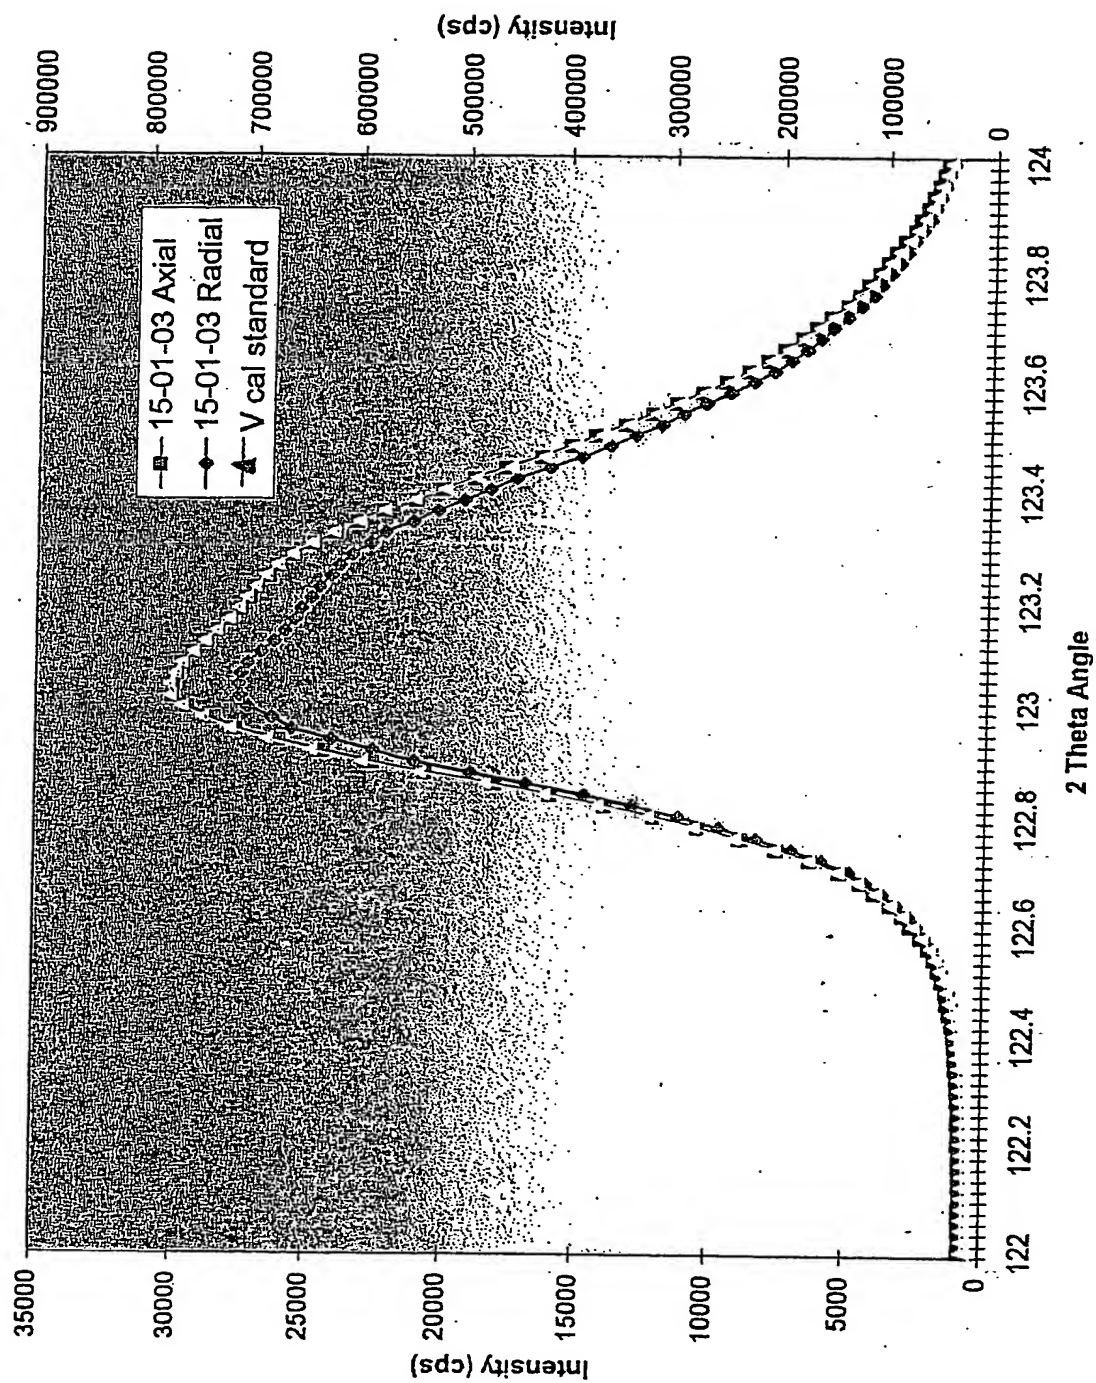


FIG. 54

15-01-03 Mn- Axial and Radial Sample vs Mn Cal Standard (LiF220/FPC)

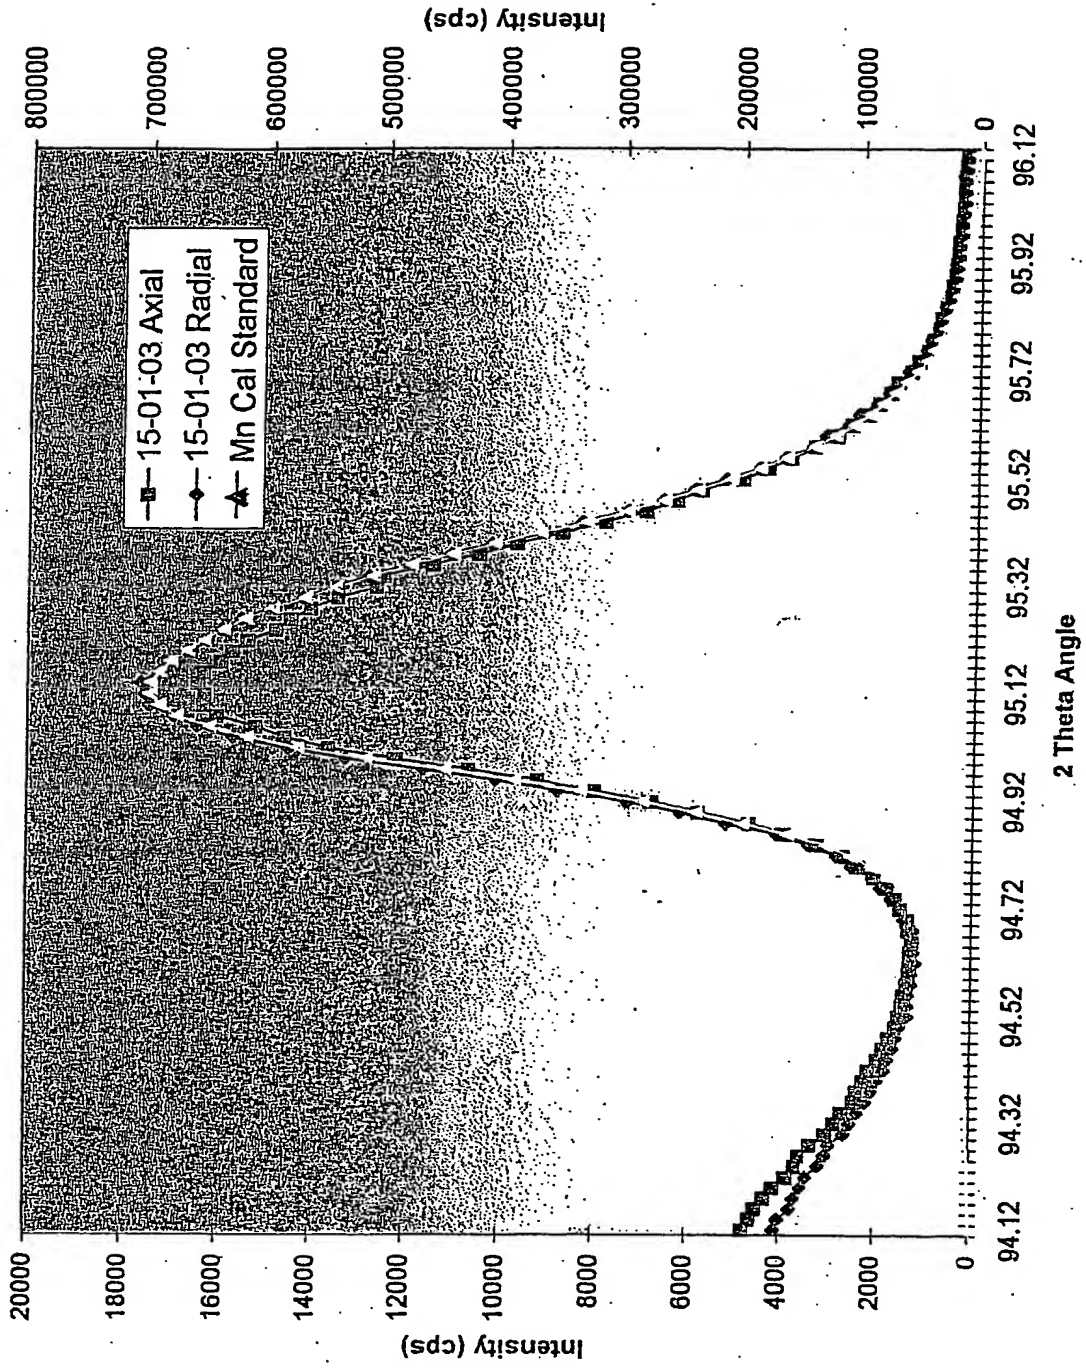


FIG. 55

15-01-03 Cube scans for Sulfur (6 Sides) Ge111/FPC

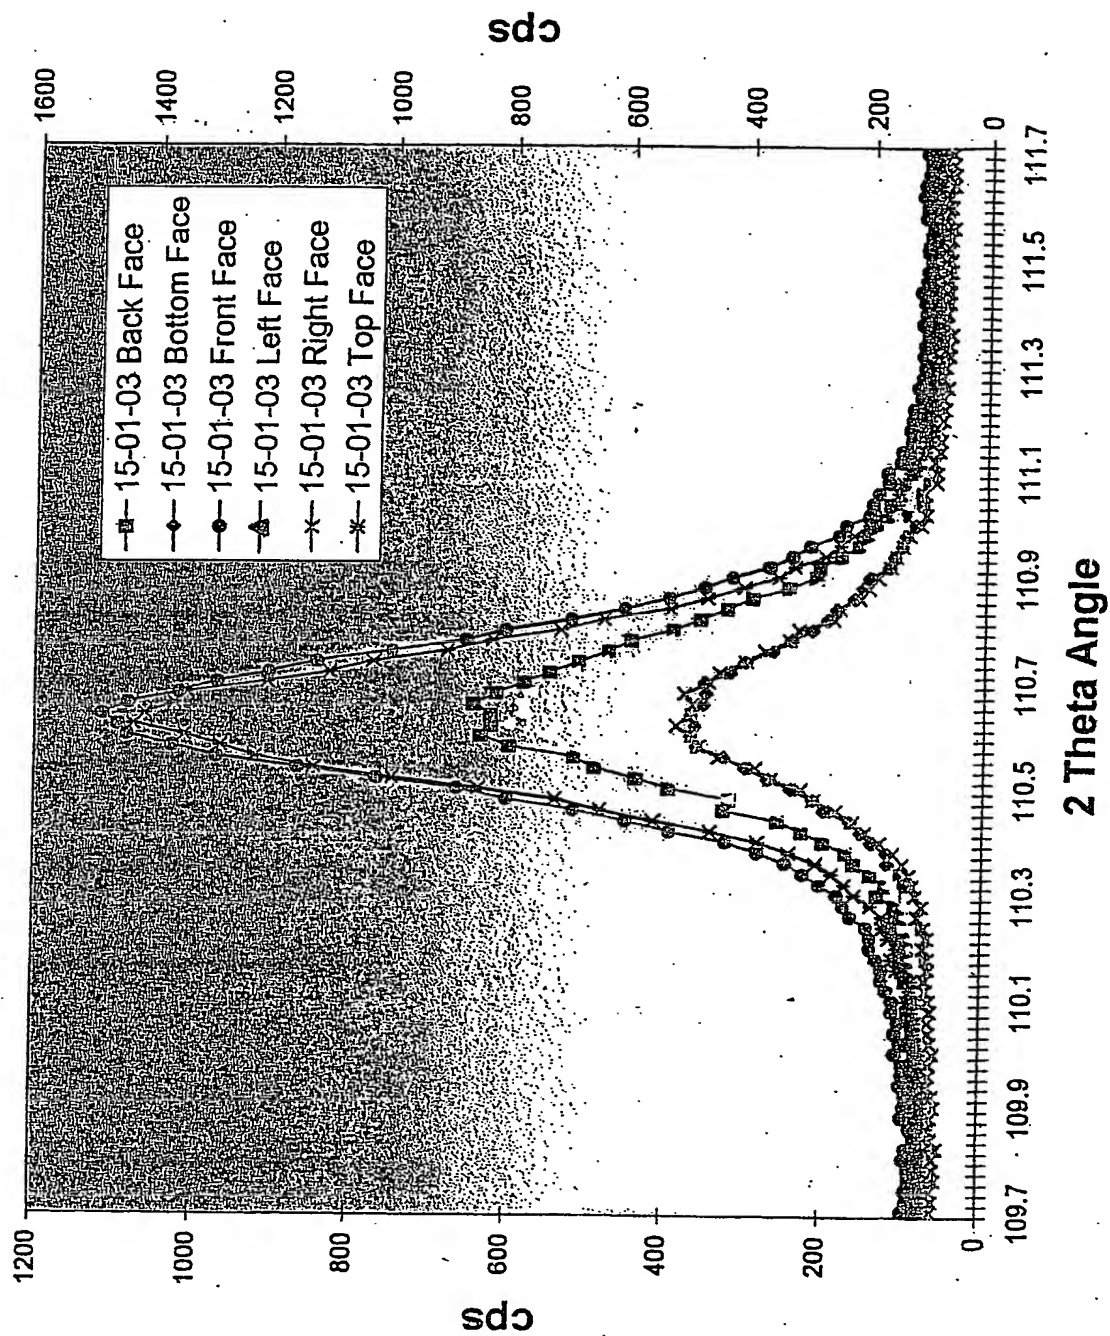


FIG. 56

15-01-04 Ta- Axial and Radial vs Ta Cal Standard

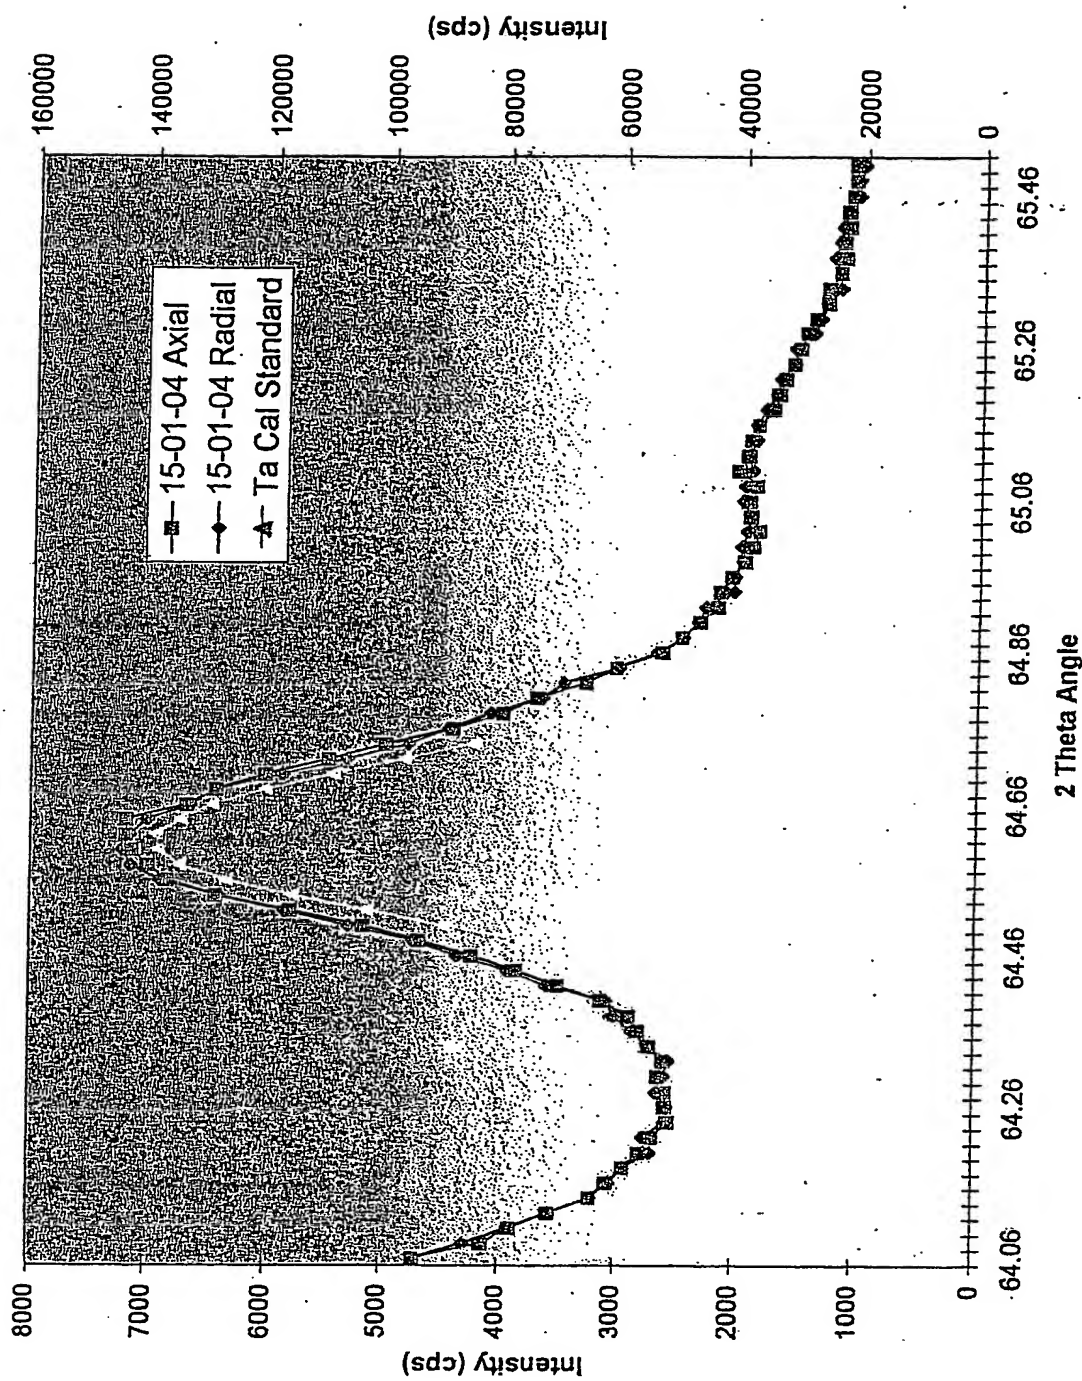


FIG. 57

15-01-04 W- Axial and Radial Samples vs W Cal Standard

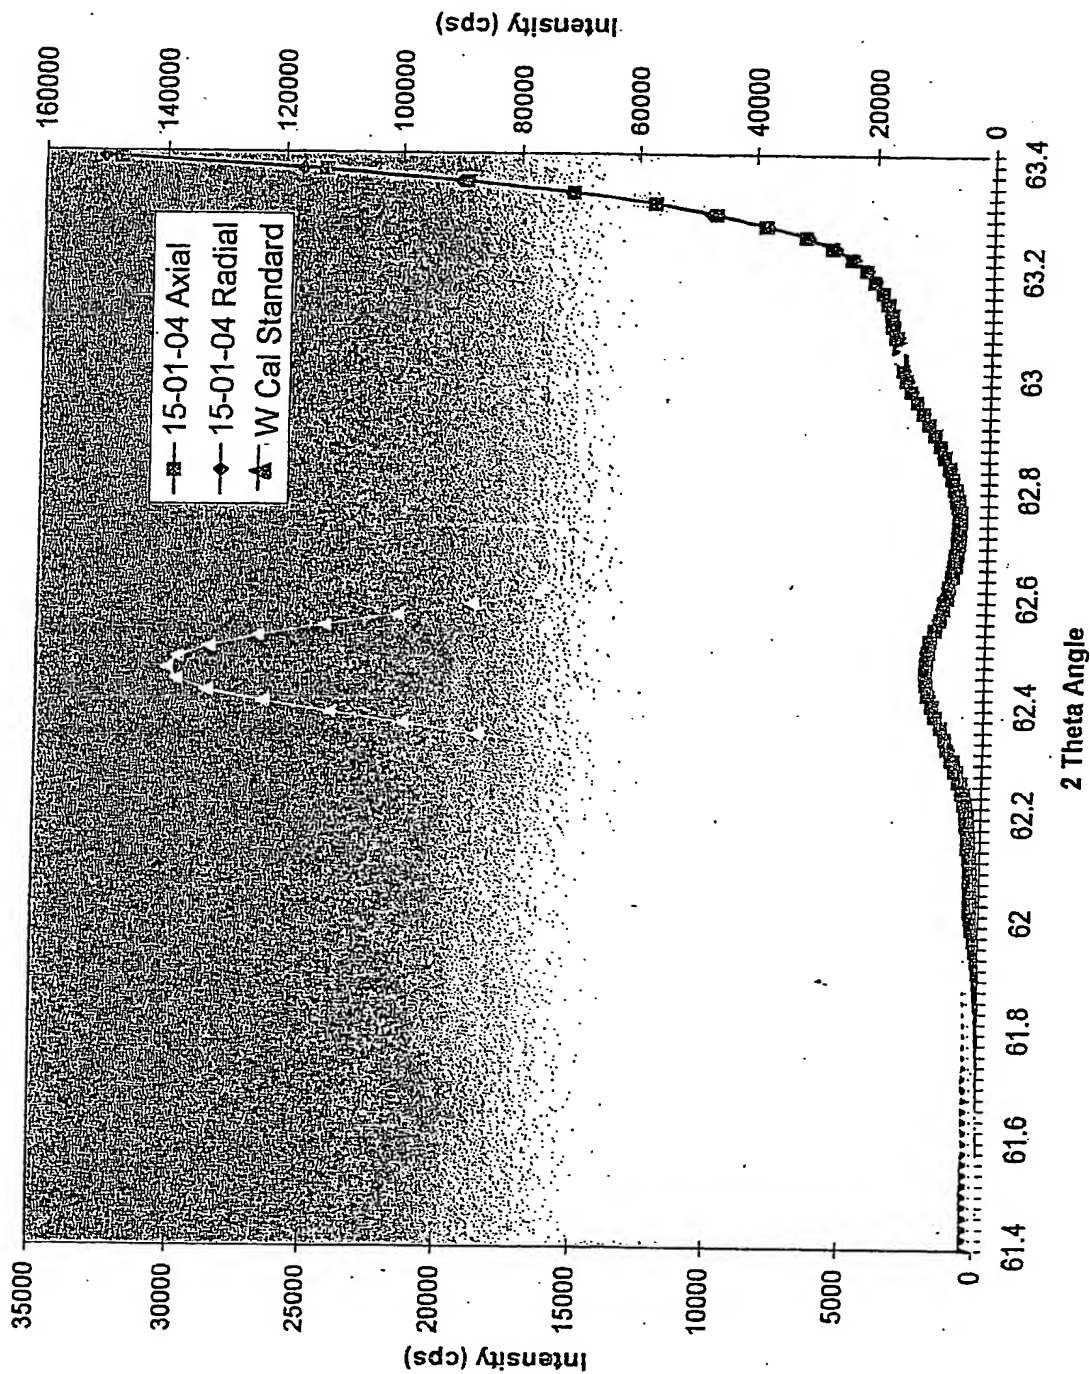


FIG. 58

15-01-04 Hf- Axial and Radial Samples vs Hf Cal Standard (LiF420/SC)

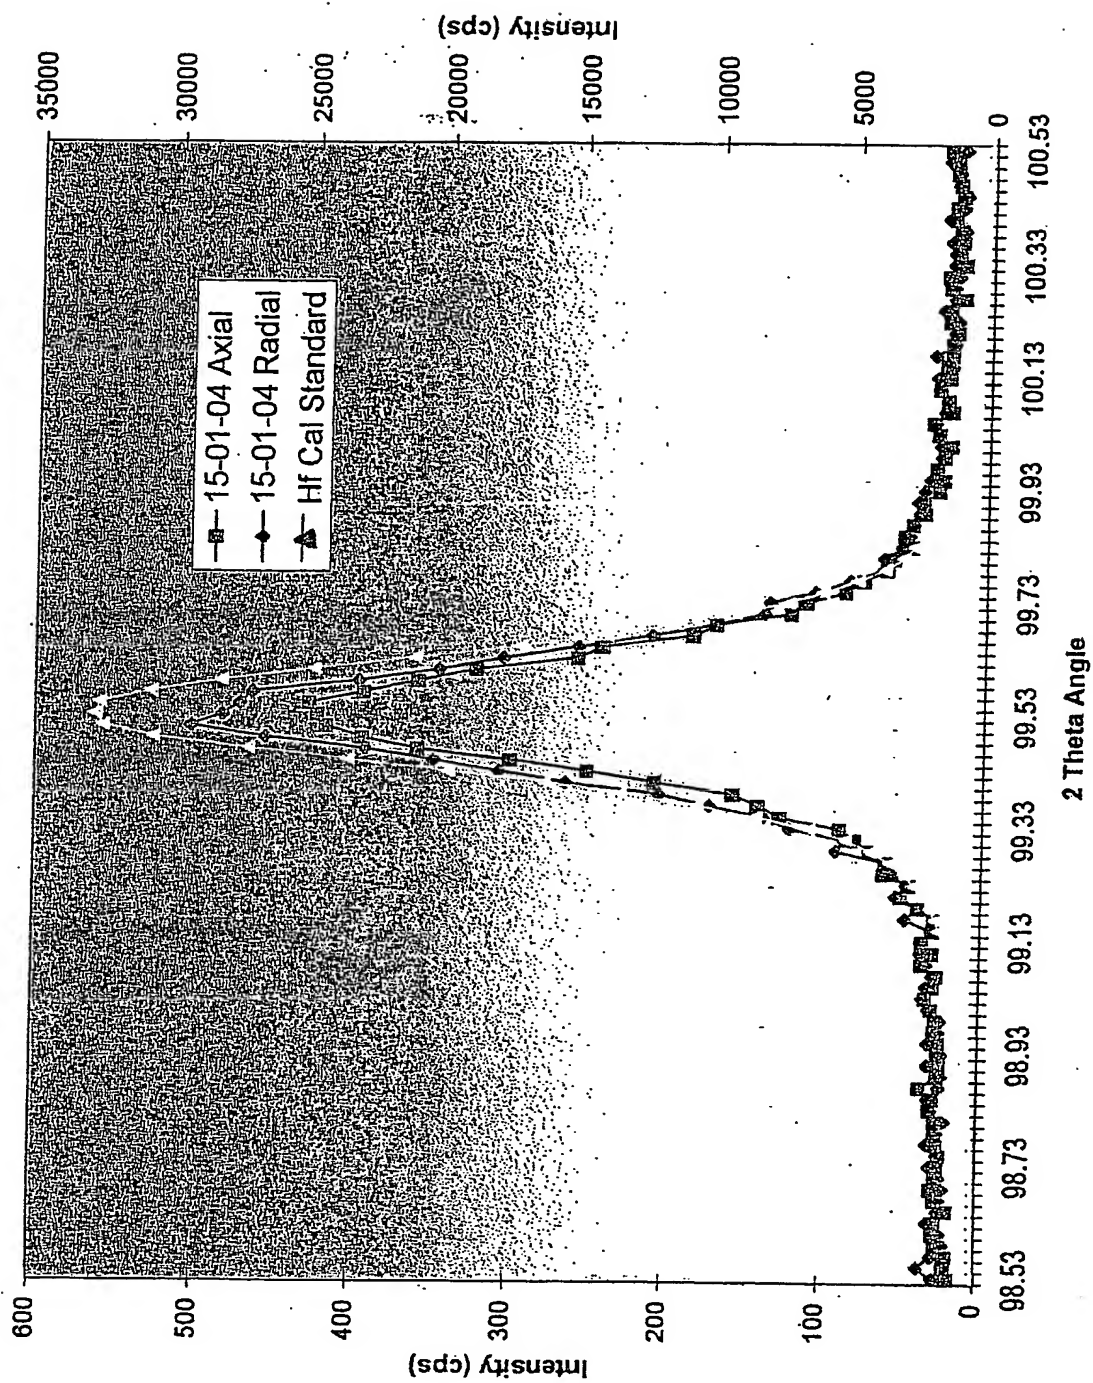


FIG. 59

XRF Scans for Sulfur (Ge111/FPC)
15-01-04 Ni/Hf/W/Ta Ingot

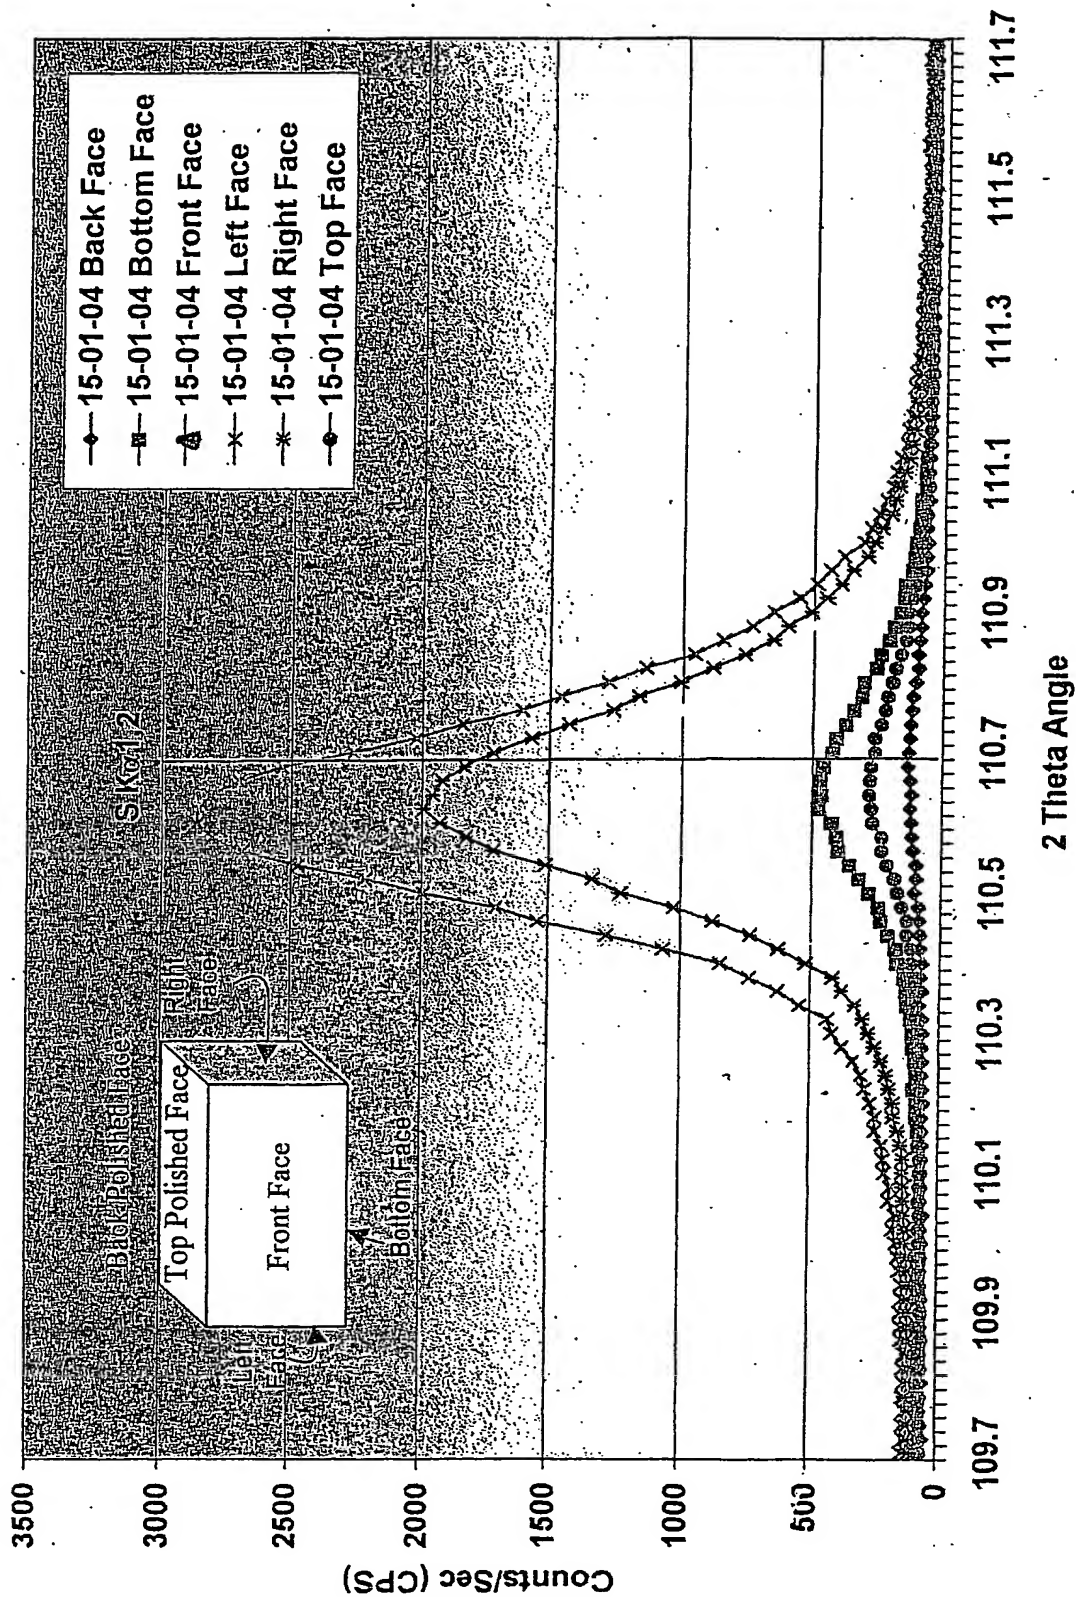


FIG. 60

15-01-04 Ni- Axial and Radial vs Ni Cal Standard (LiF220/FPC)


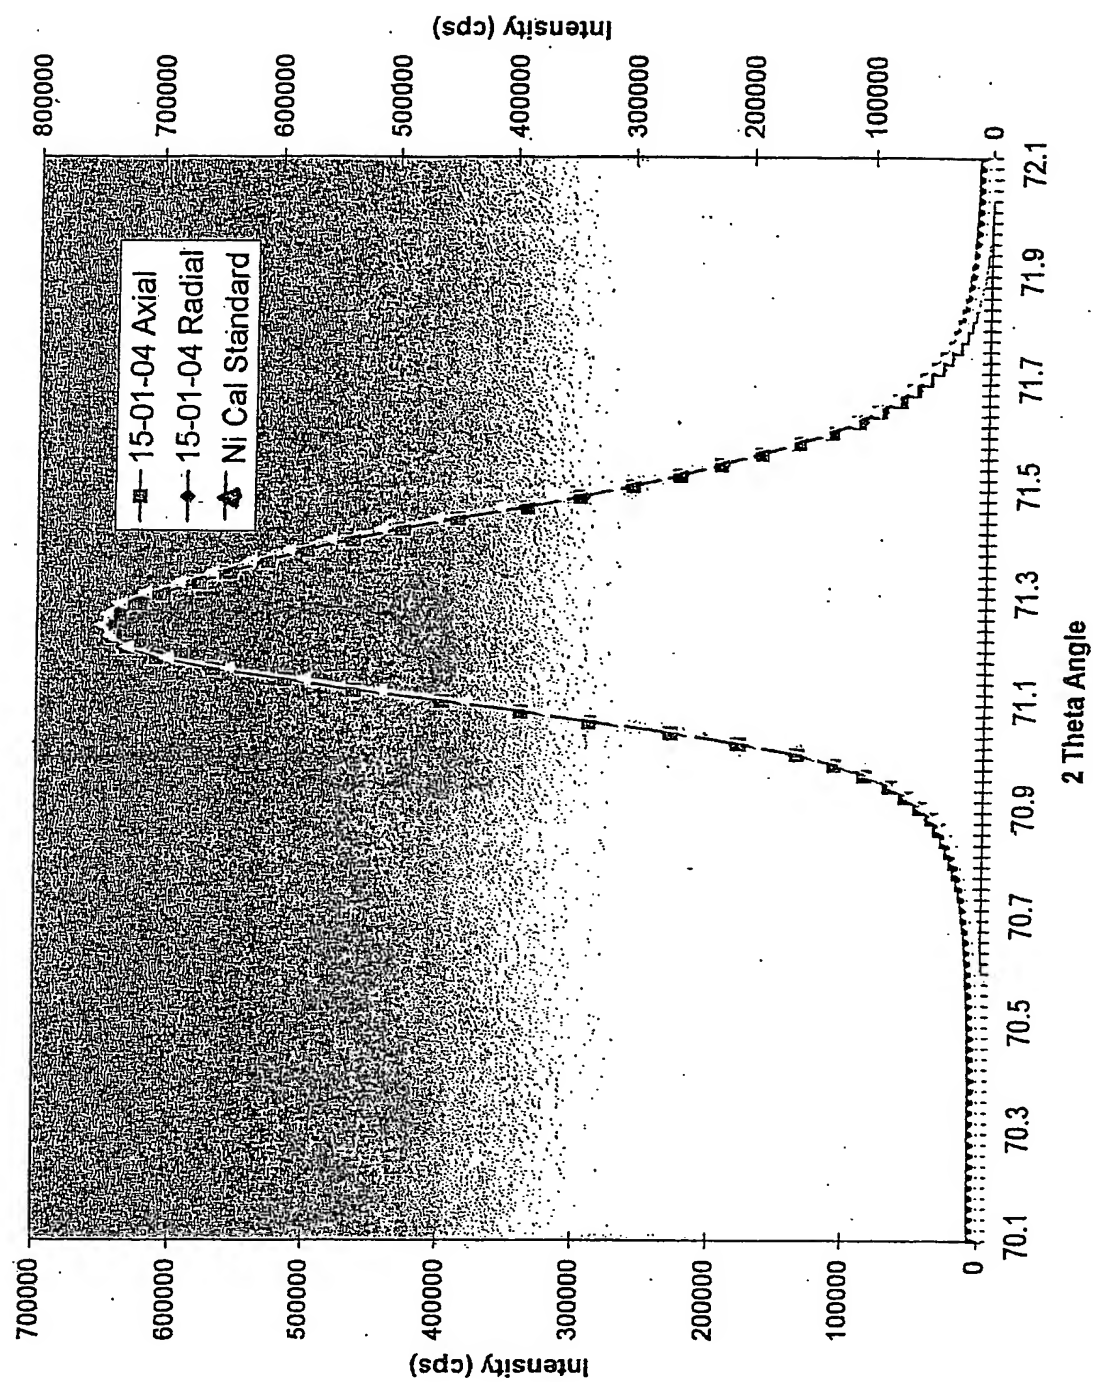


FIG. 61

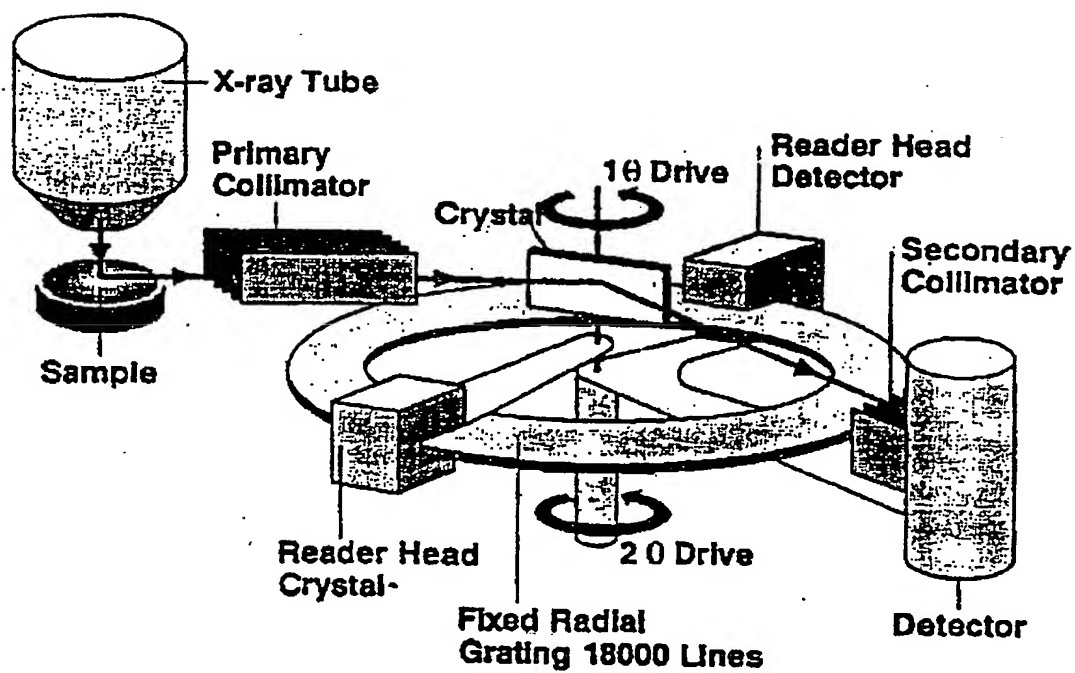

Schematic layout of ARL 8410 sequential XRF.

FIG. 62